

RECEIVED

JUL 26 2001

TC 1700 MAIL ROOM
BLOOD ETHANOL

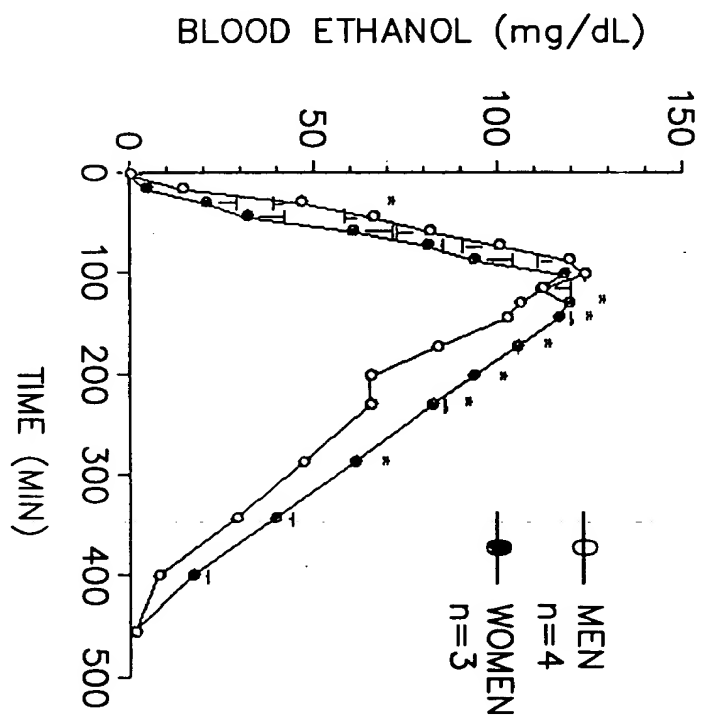
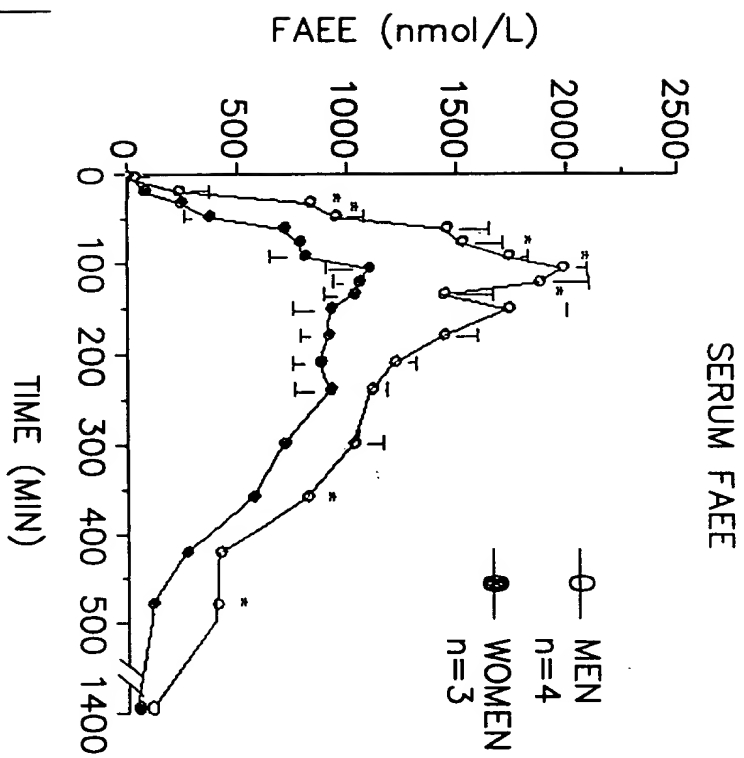


FIG. 1

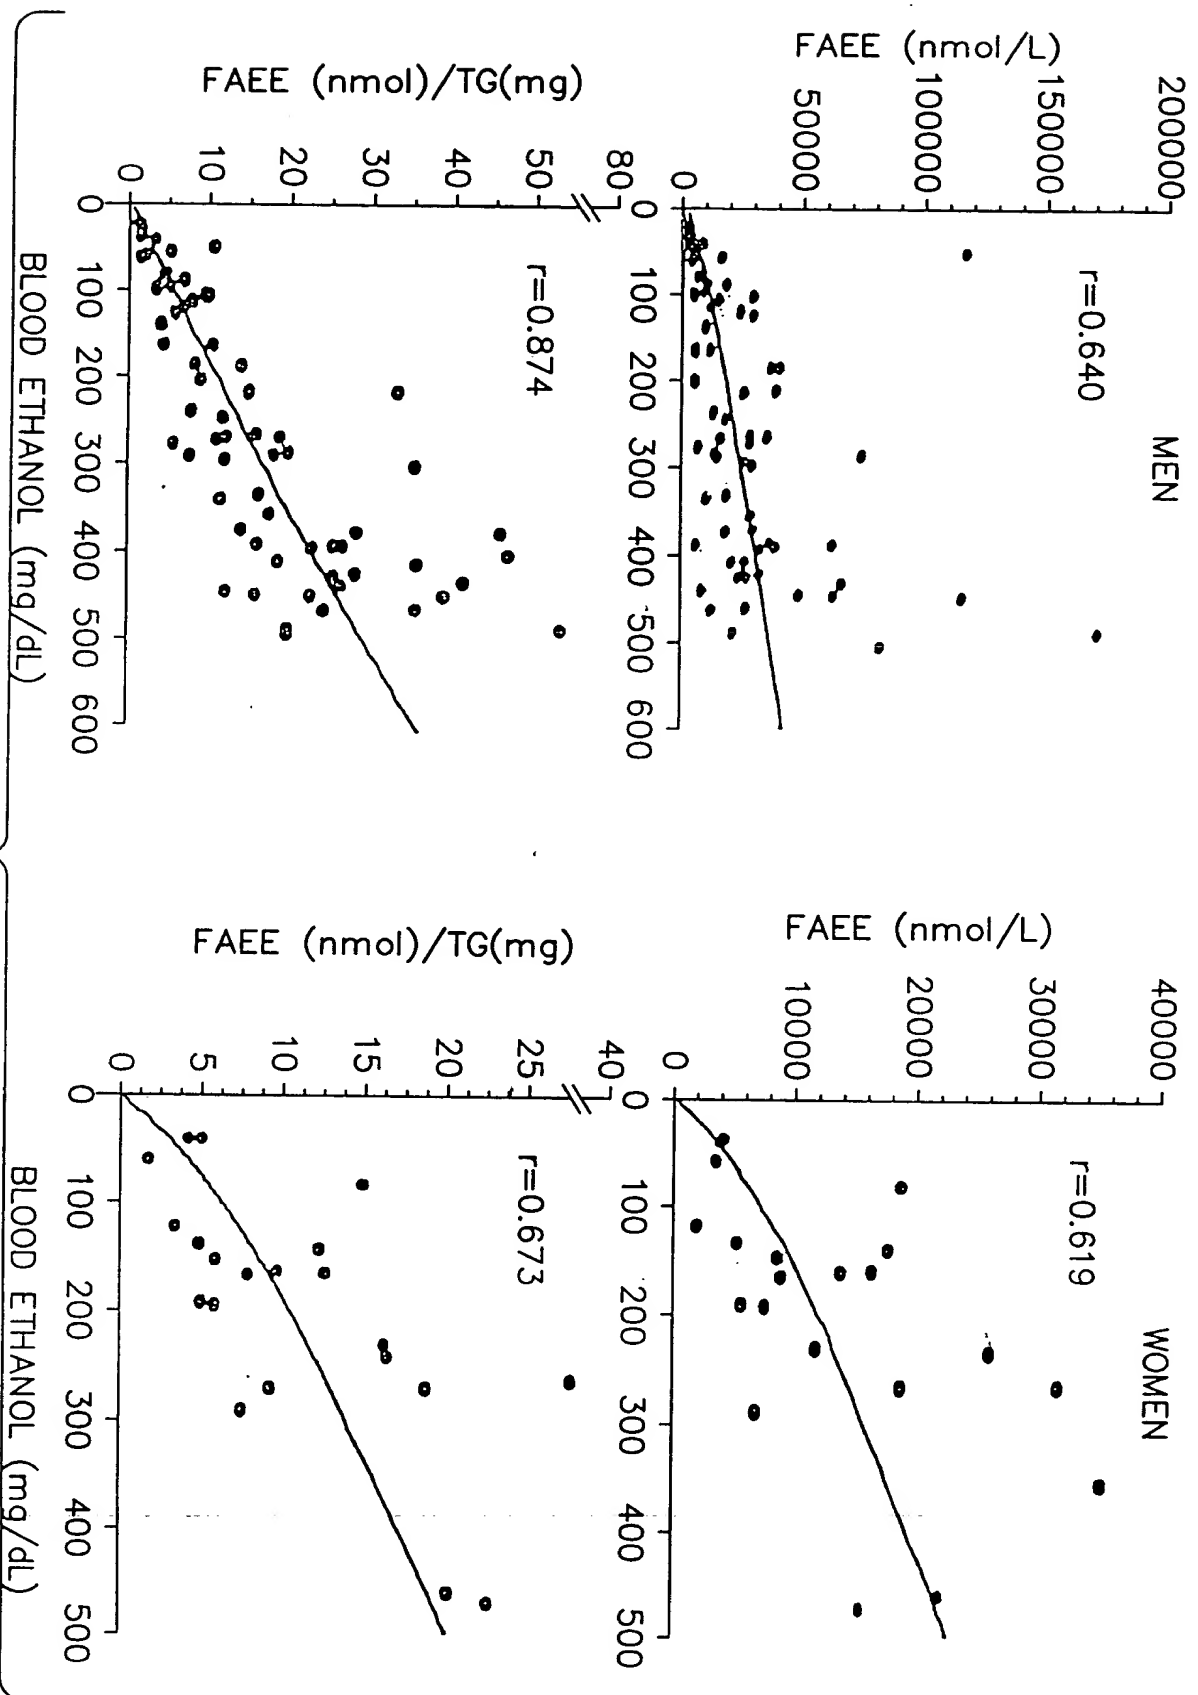


FIG. 2

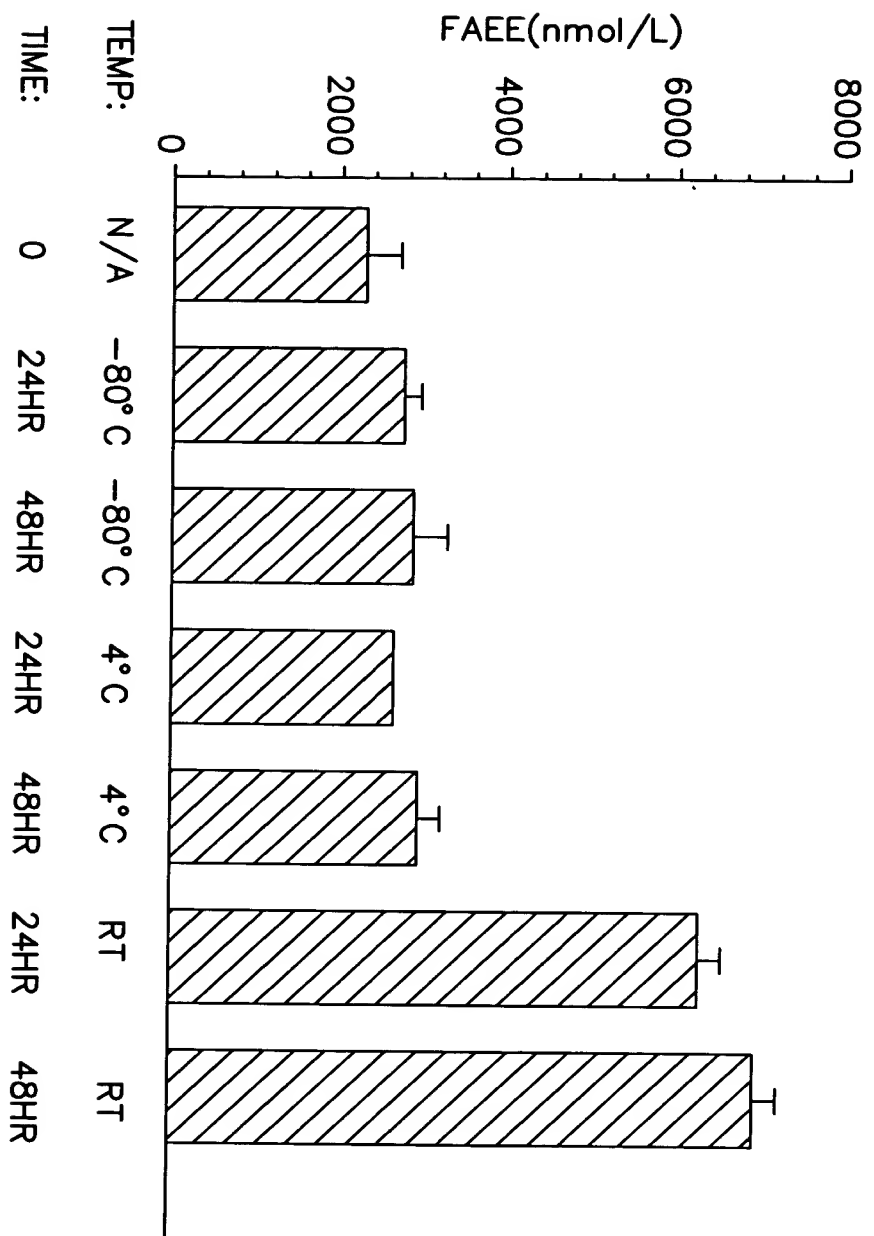


FIG. 3

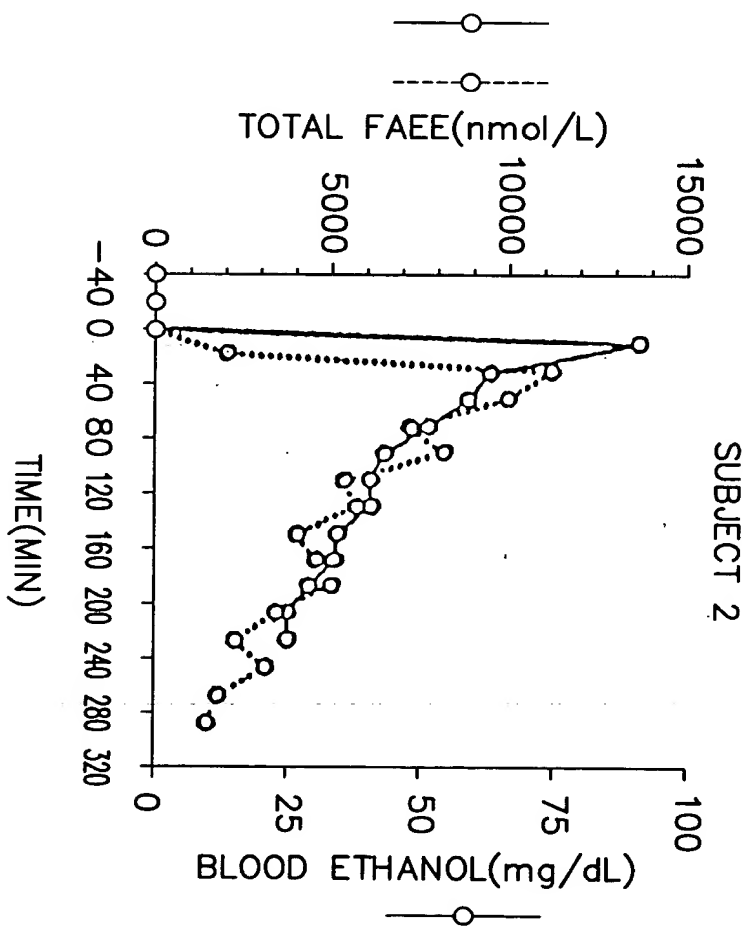
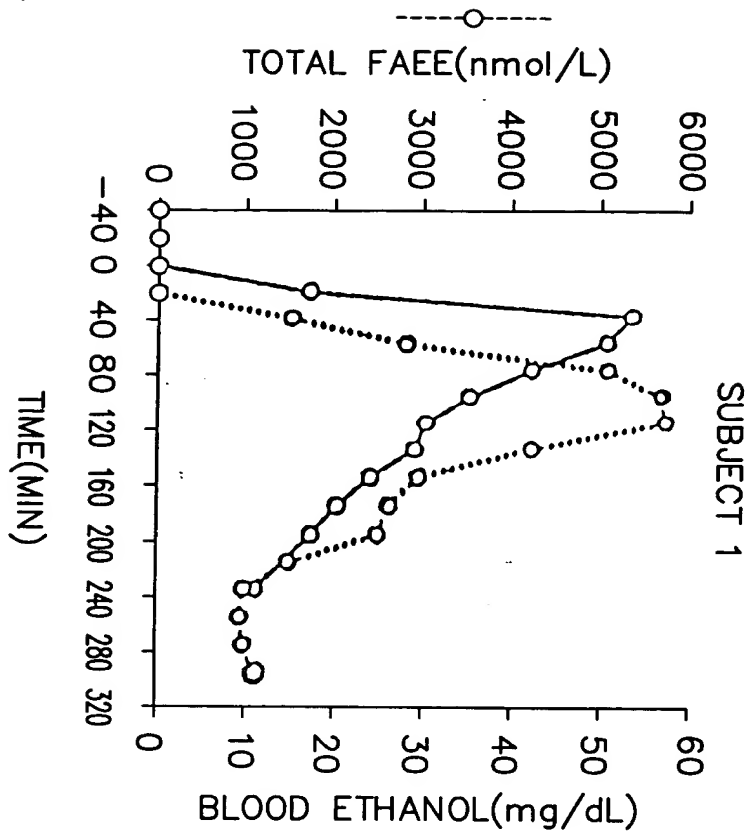


FIG. 4A

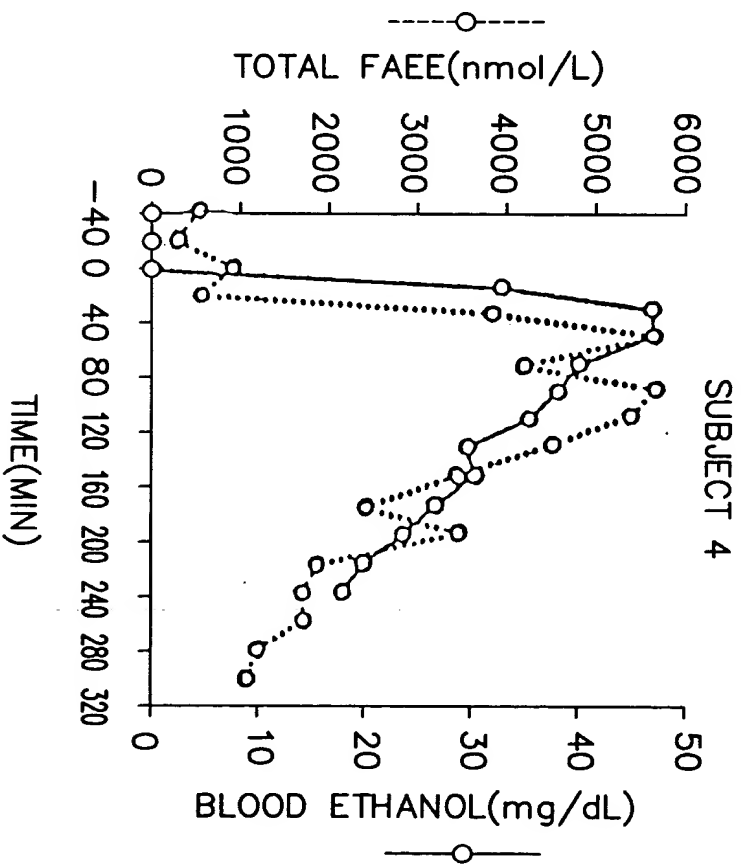
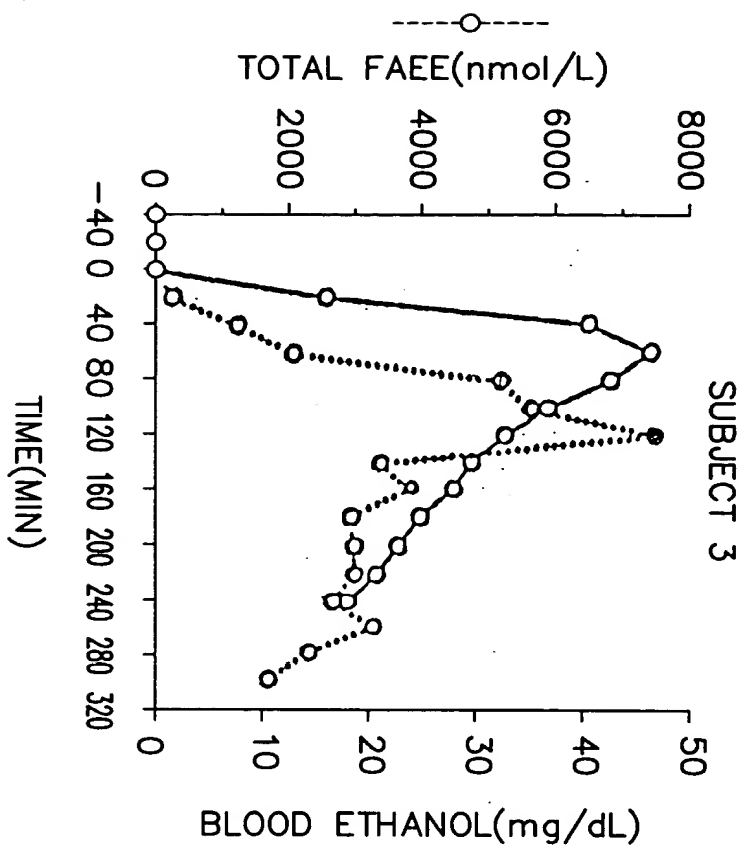


FIG. 4B

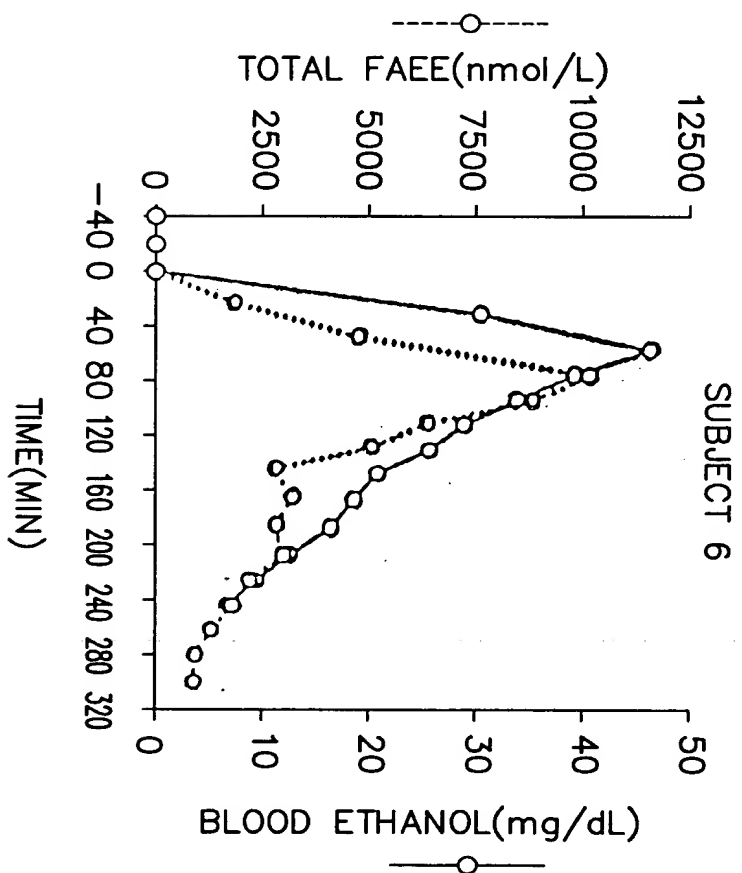
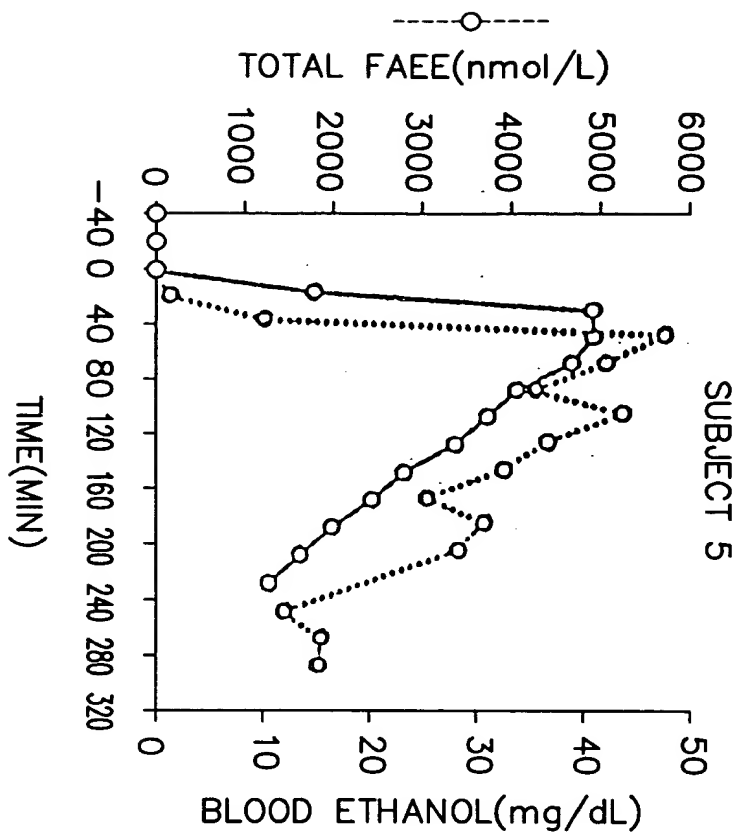


FIG. 4C

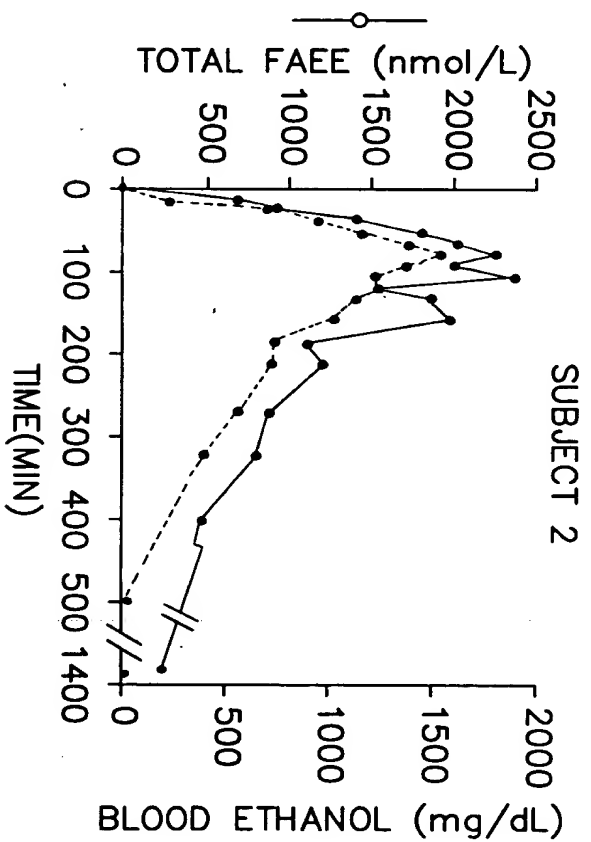
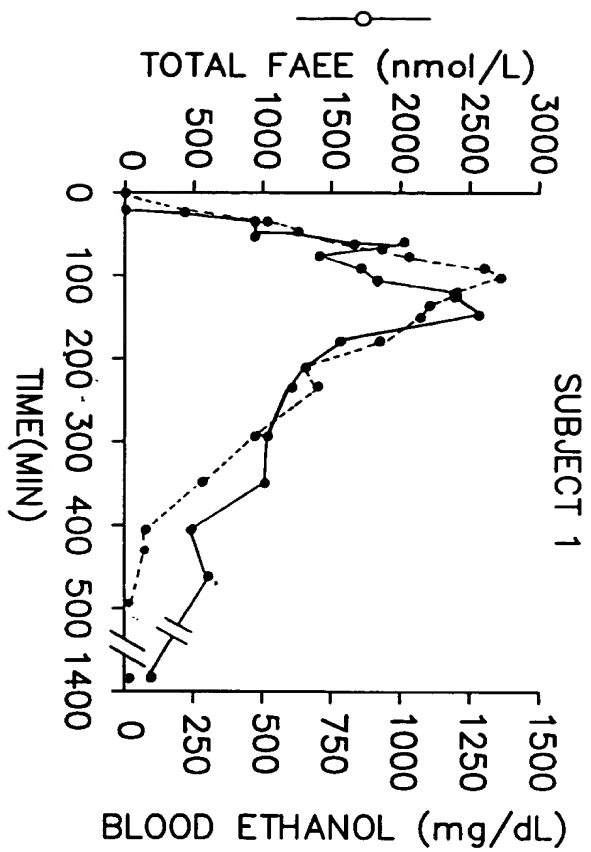


FIG. 5A

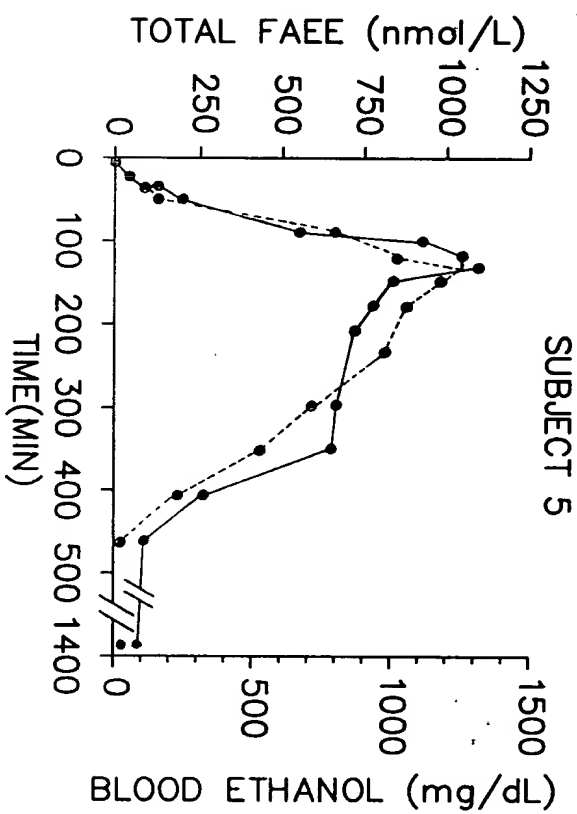
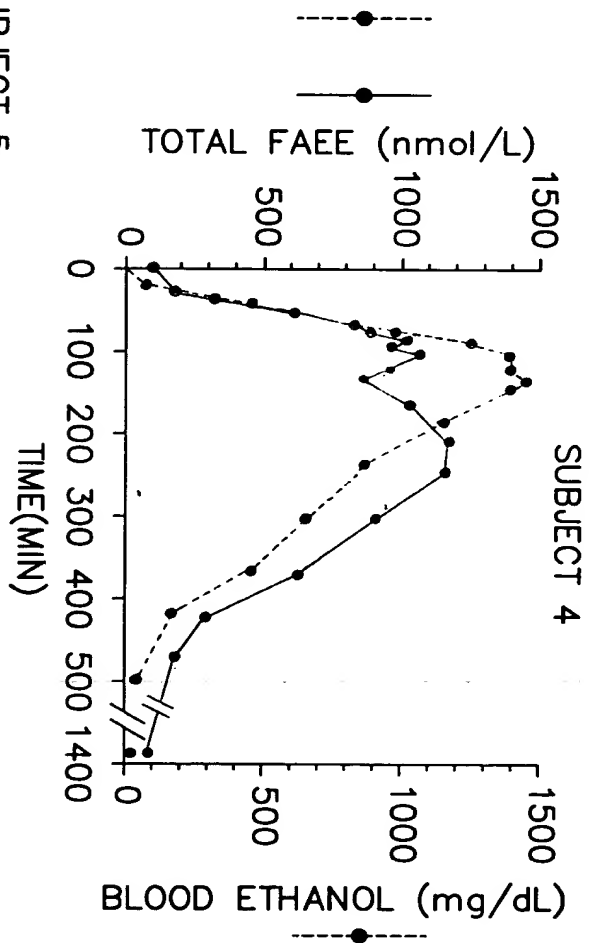
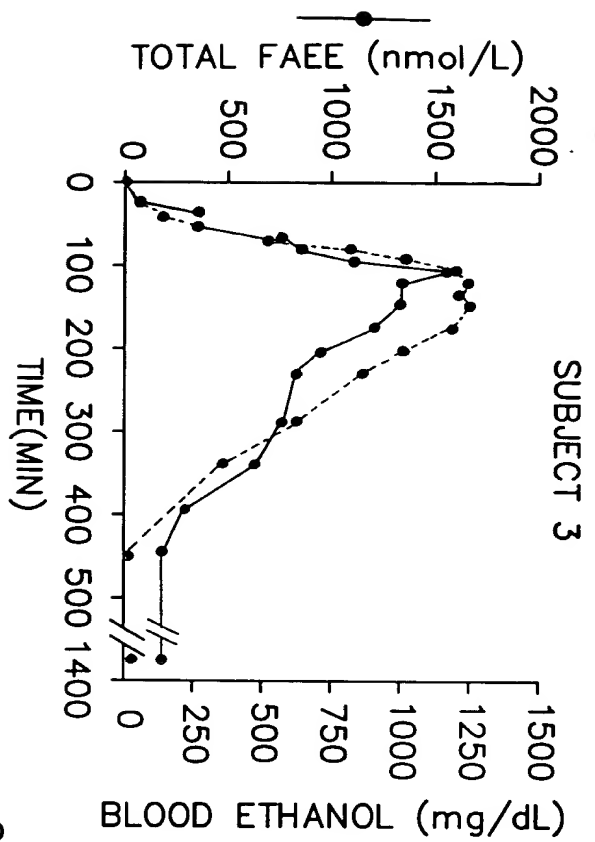


FIG. 5B

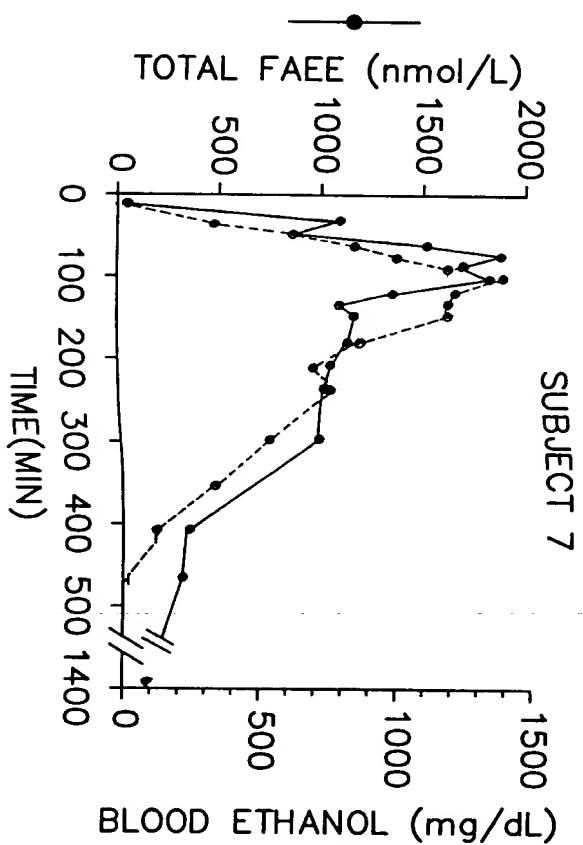
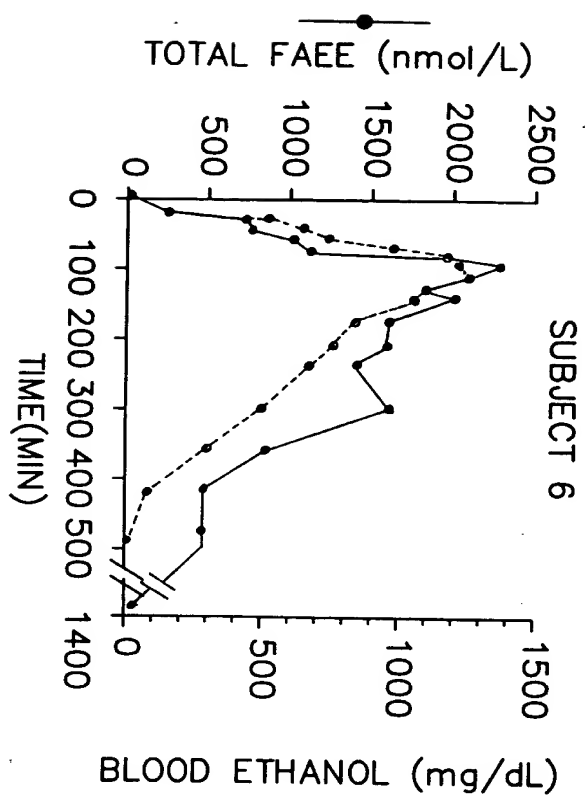


FIG. 5C

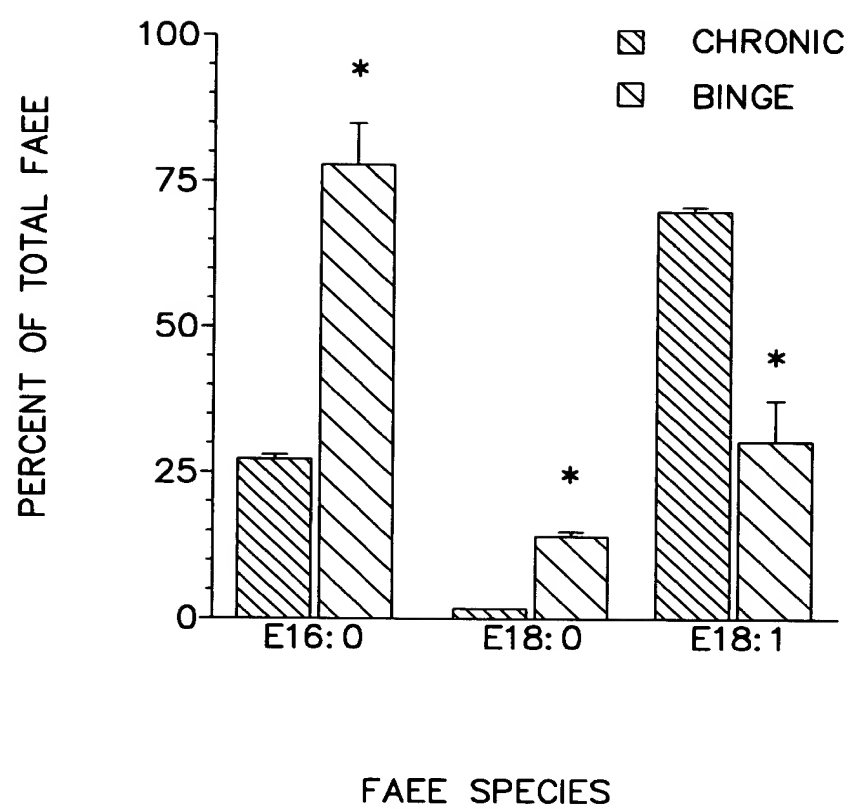


FIG. 6

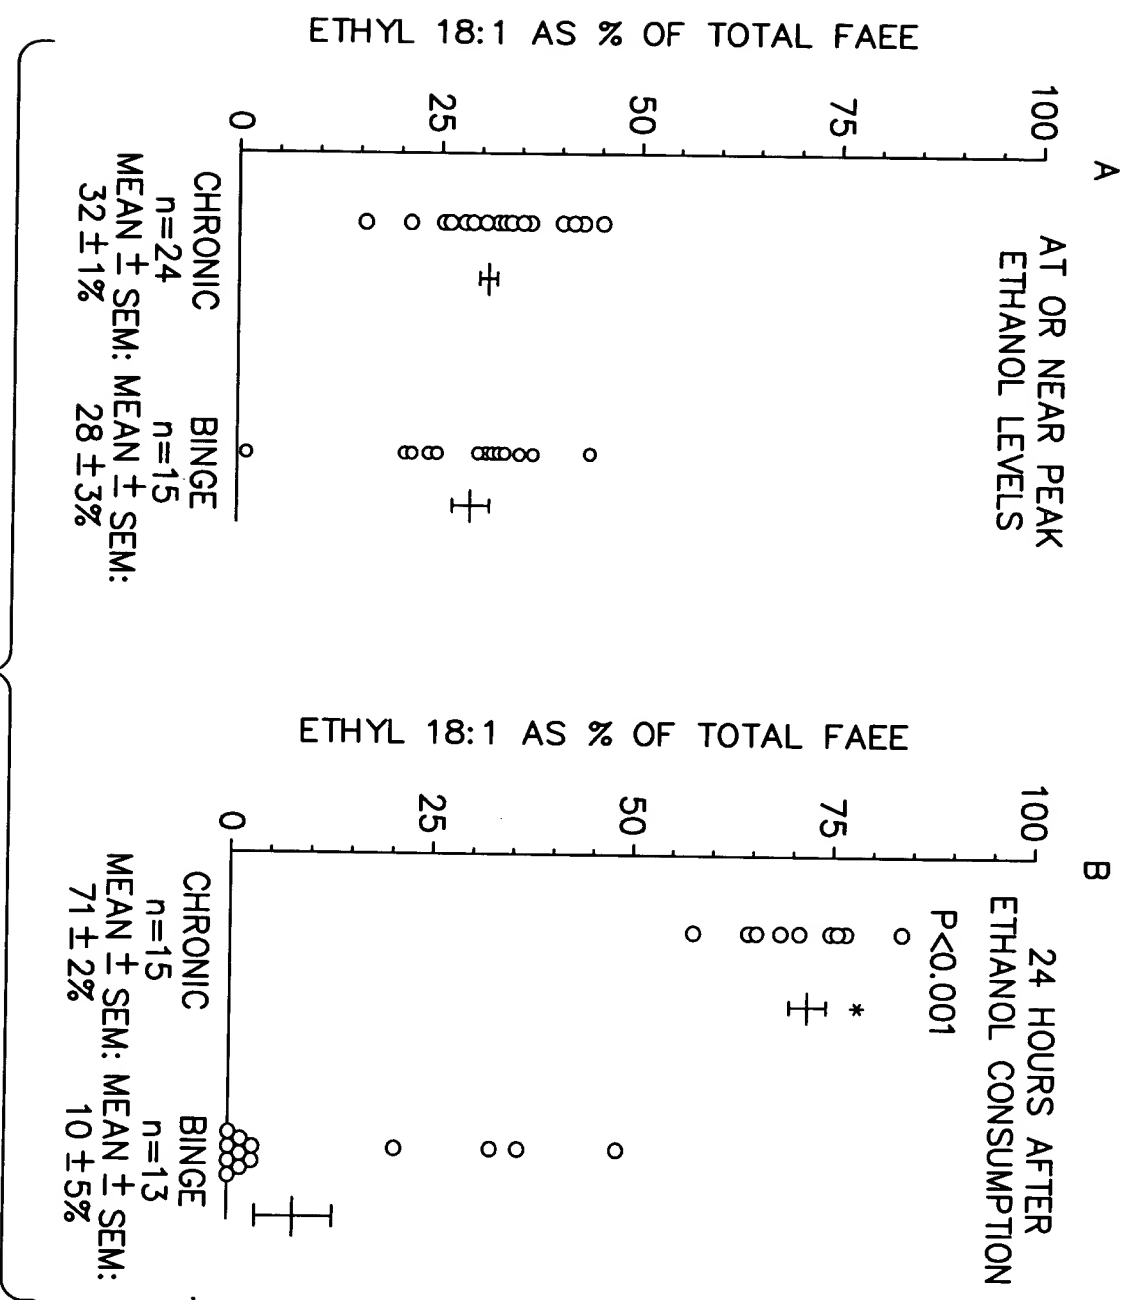


FIG. 7

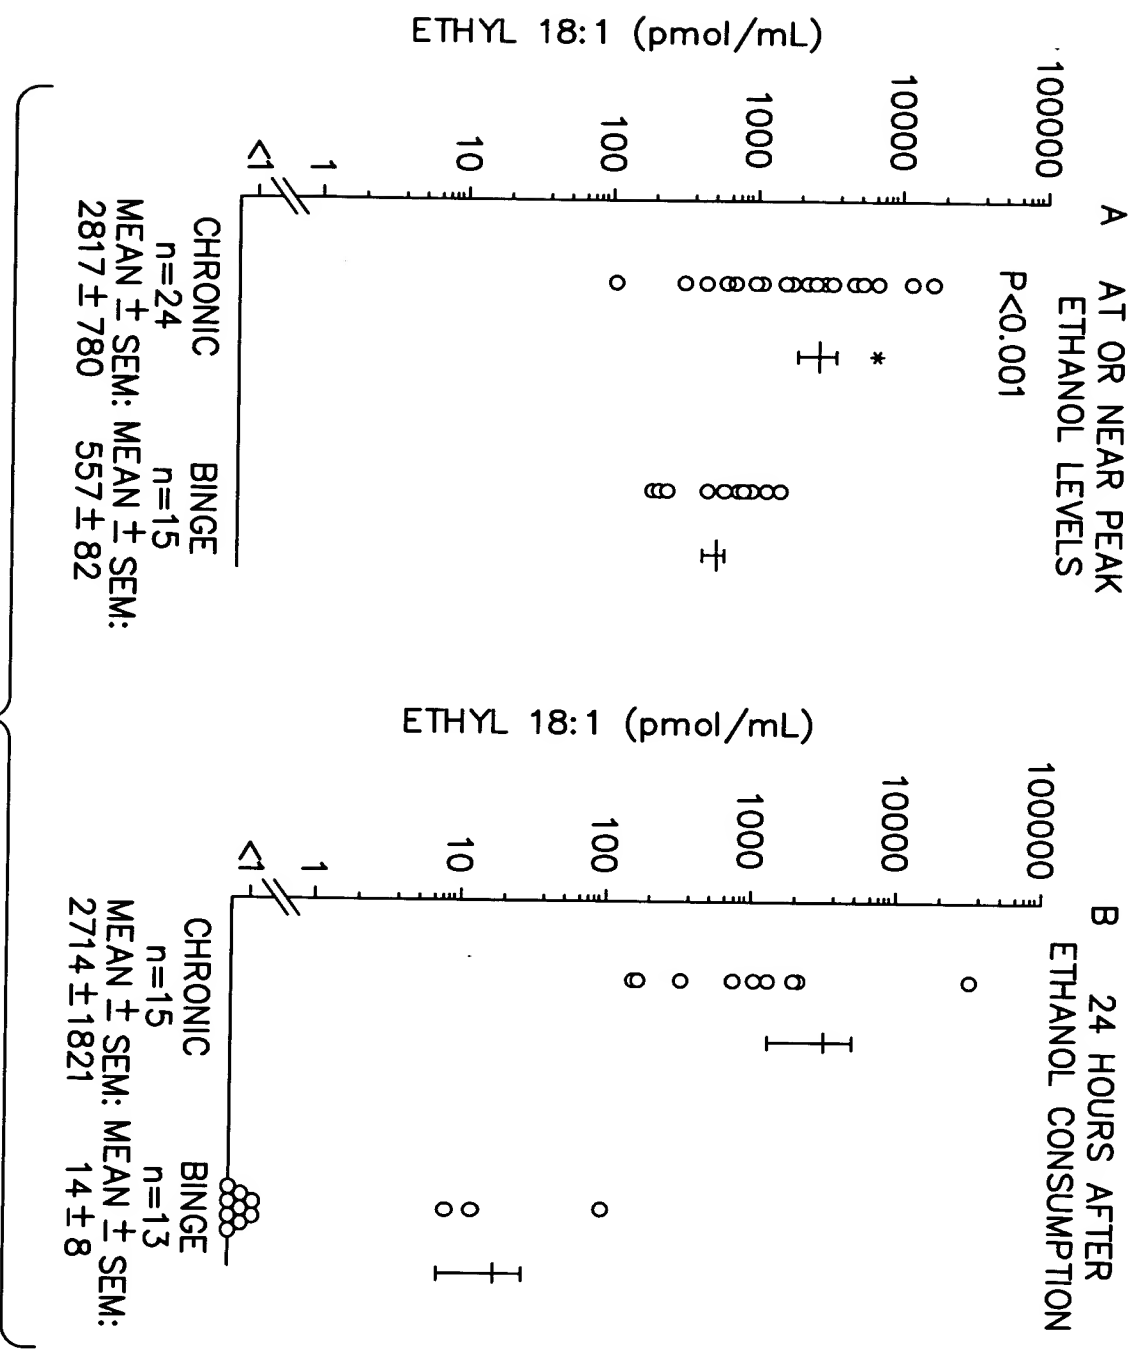


FIG. 8

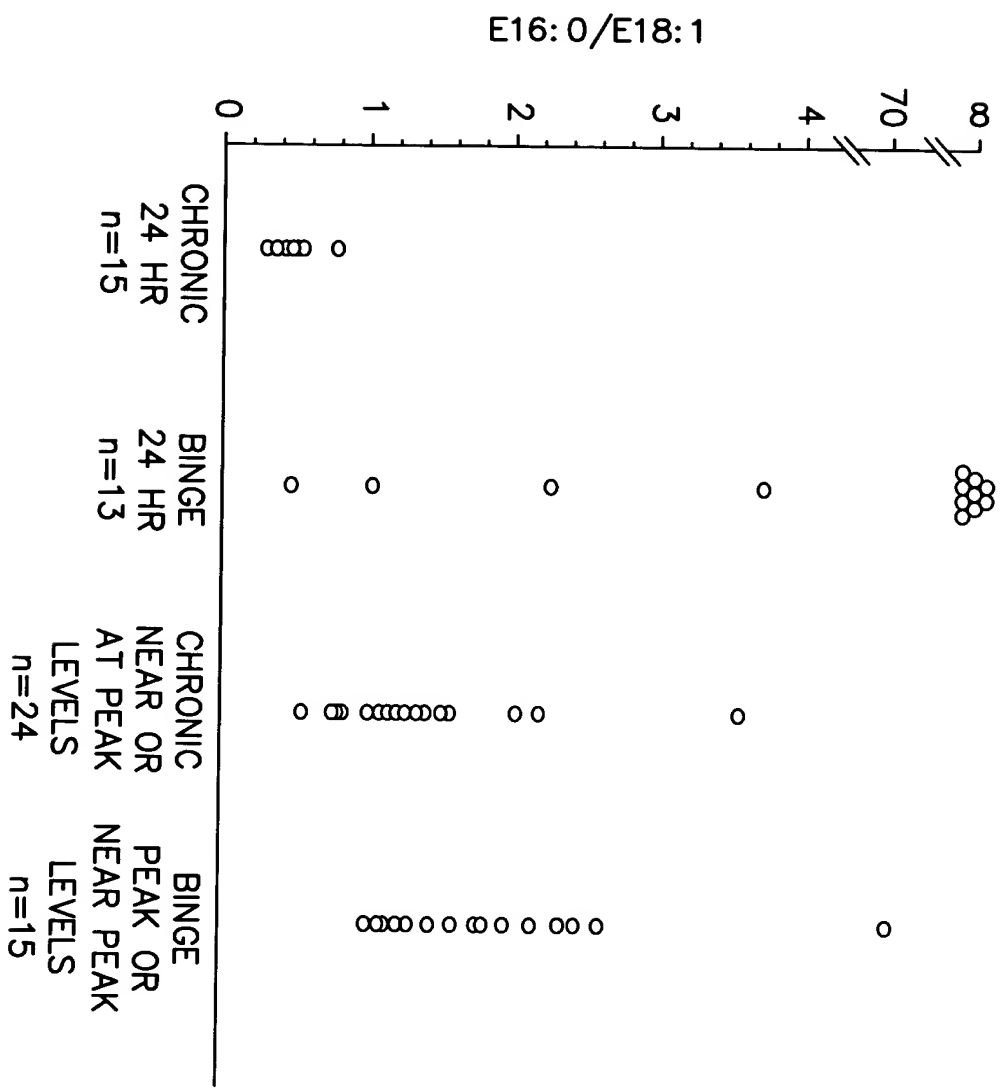


FIG. 9

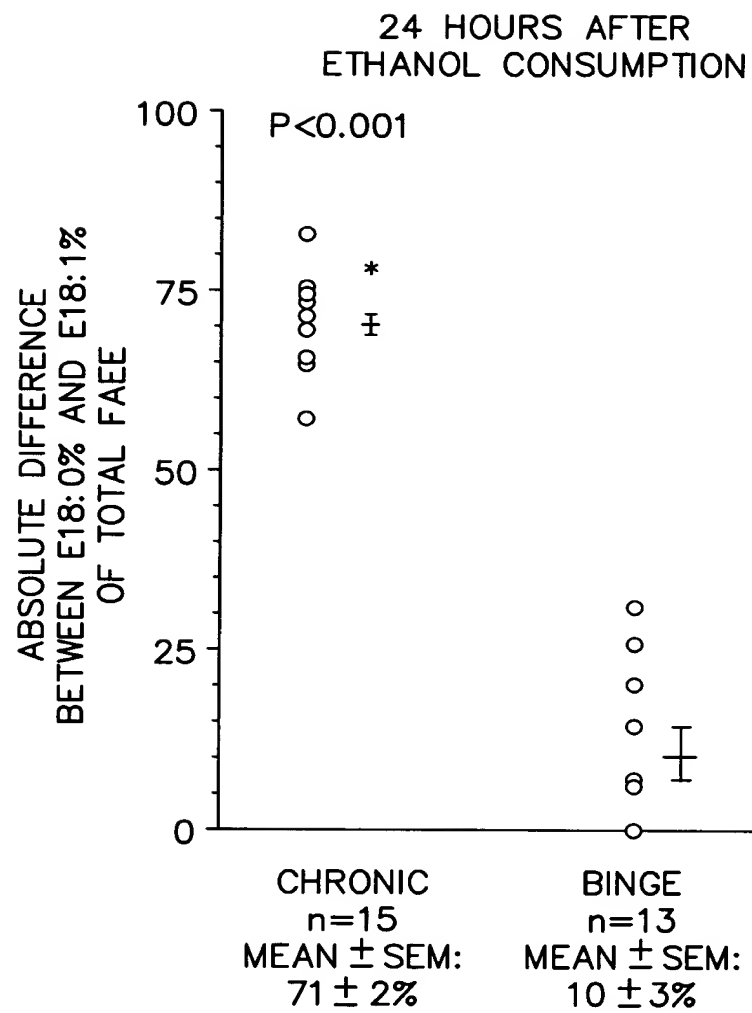


FIG. 10

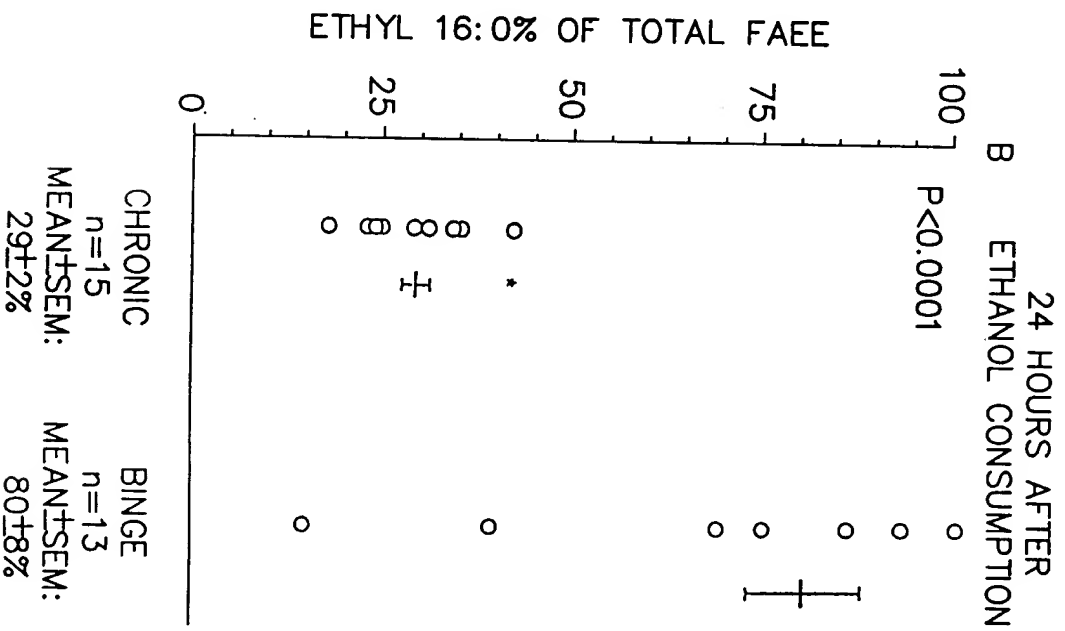
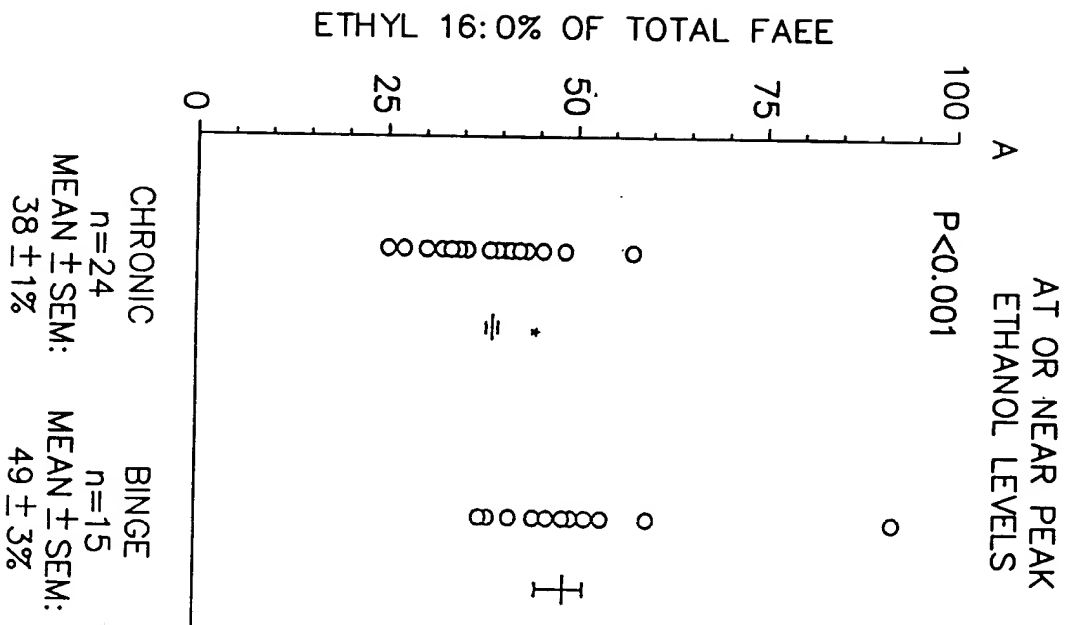


FIG. 11

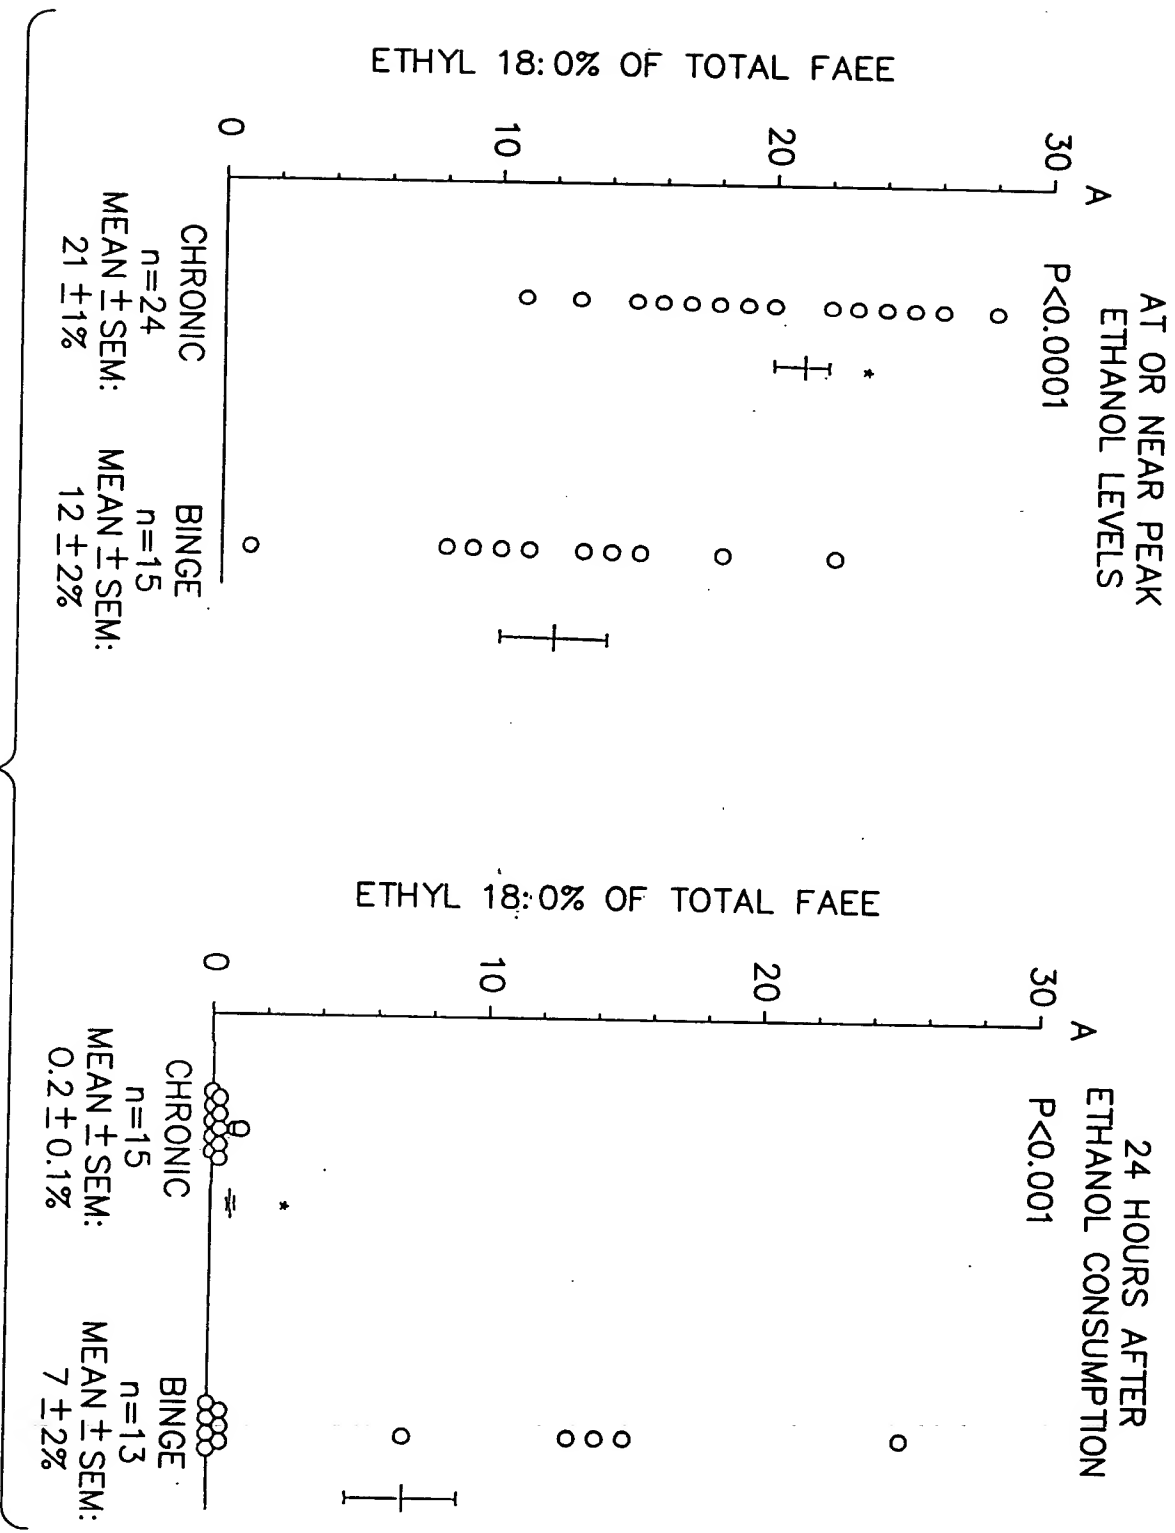


FIG. 12

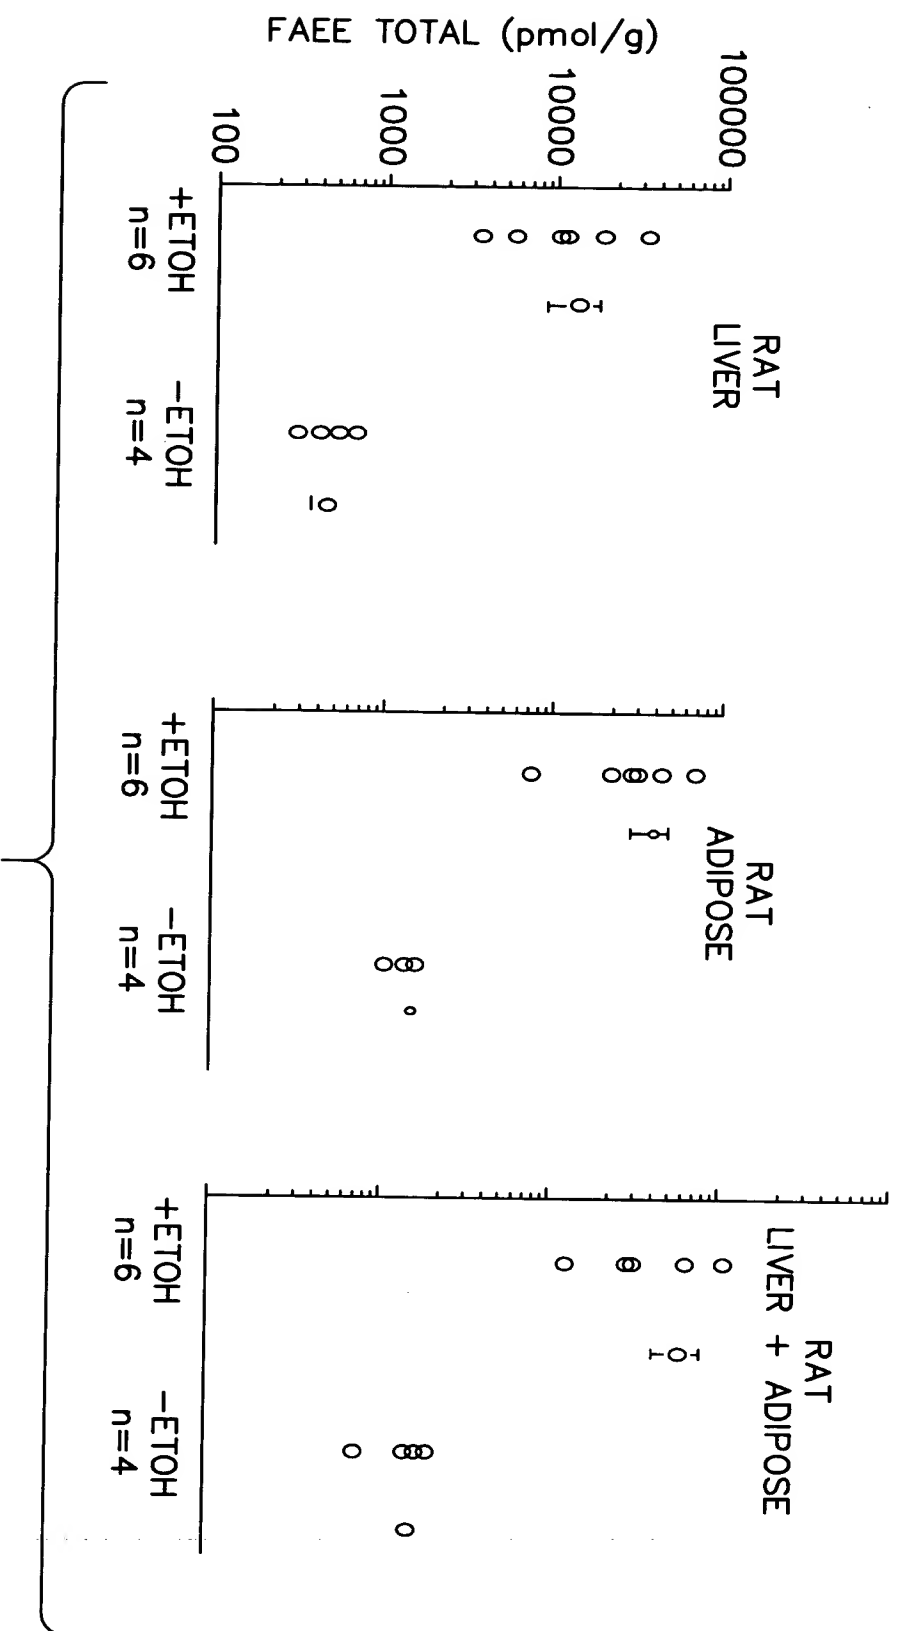


FIG. 13

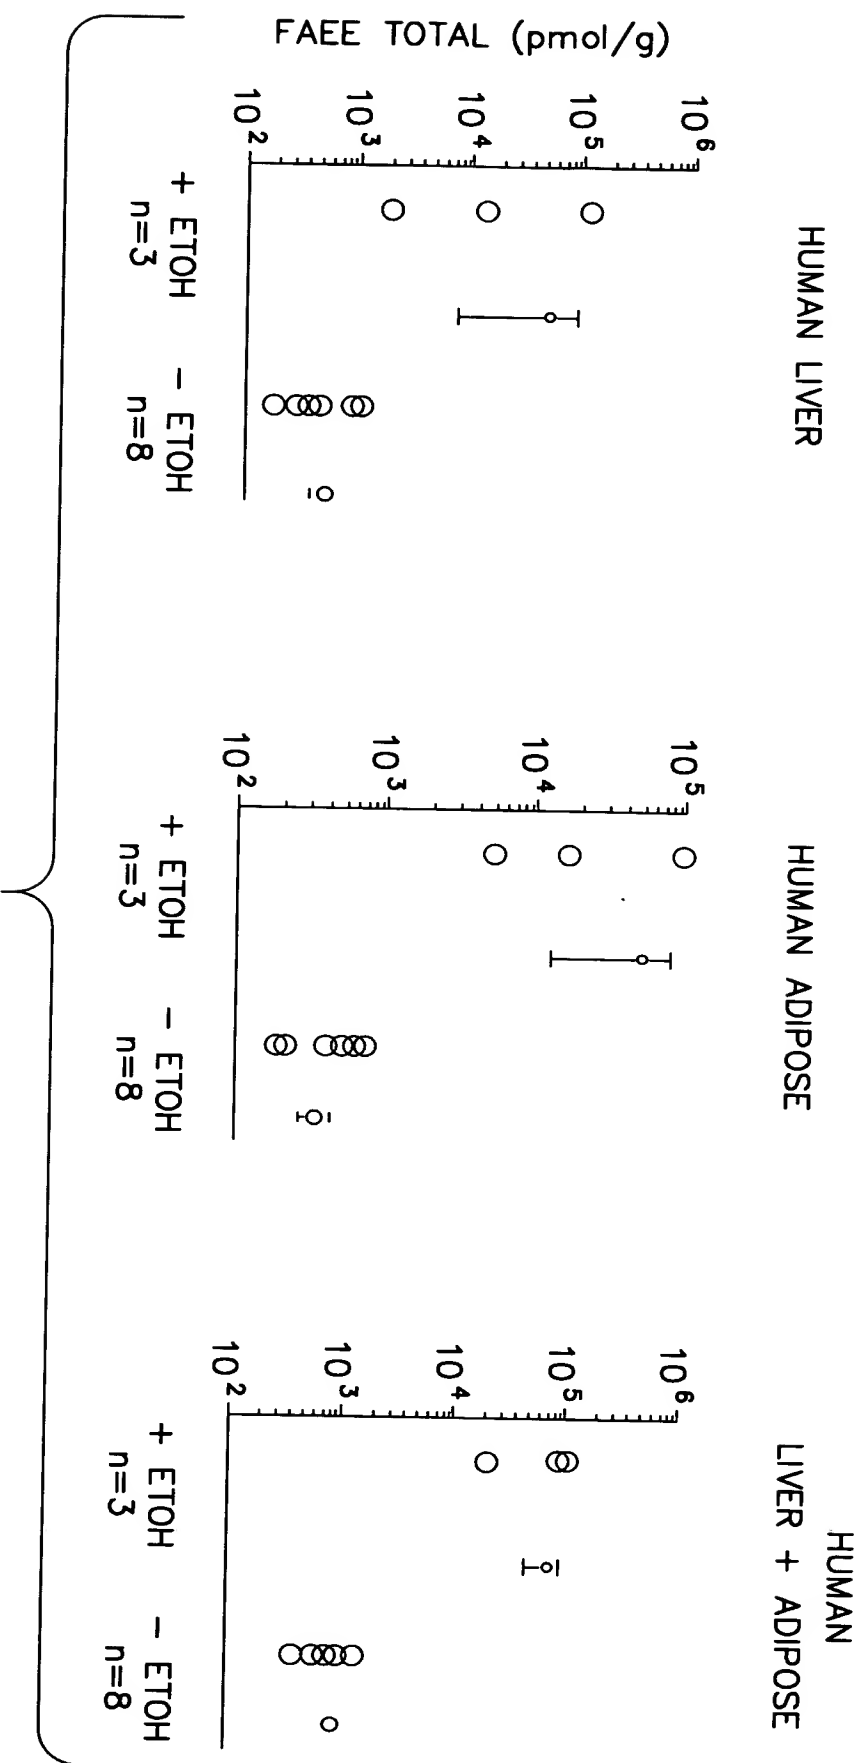


FIG. 14

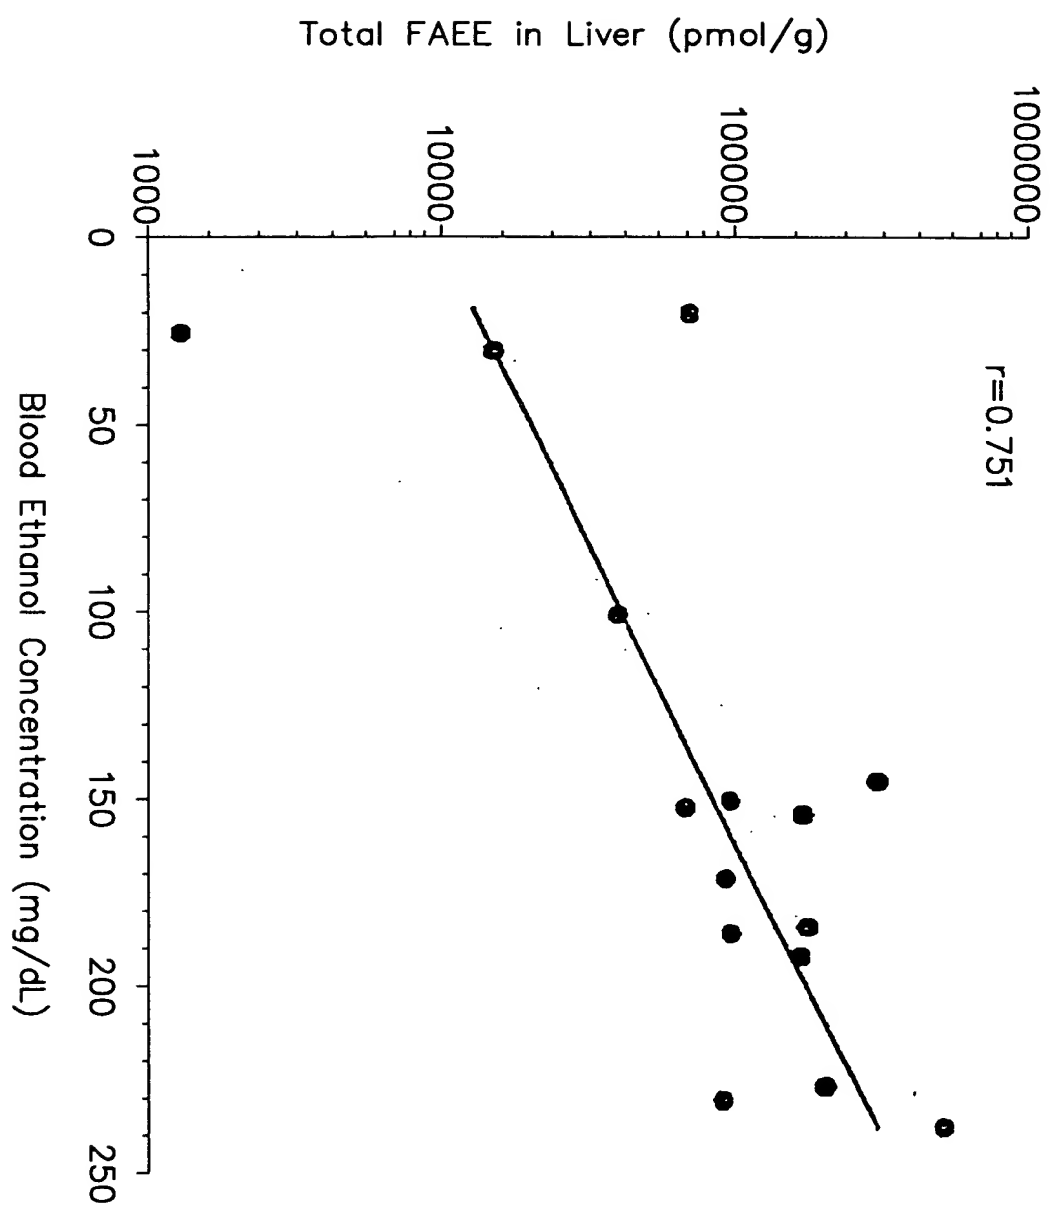


FIG. 15

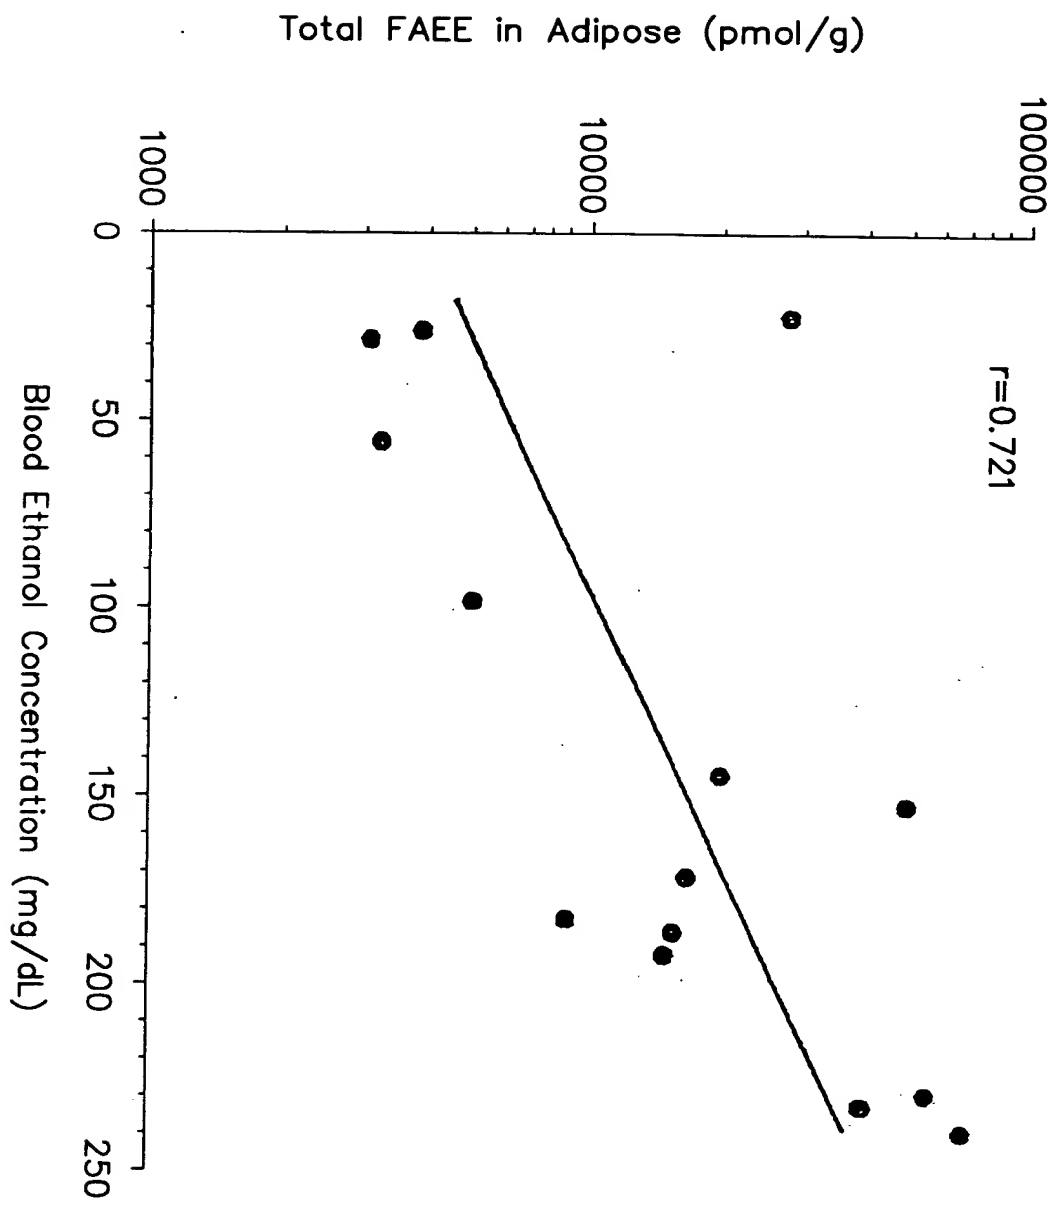


FIG. 16

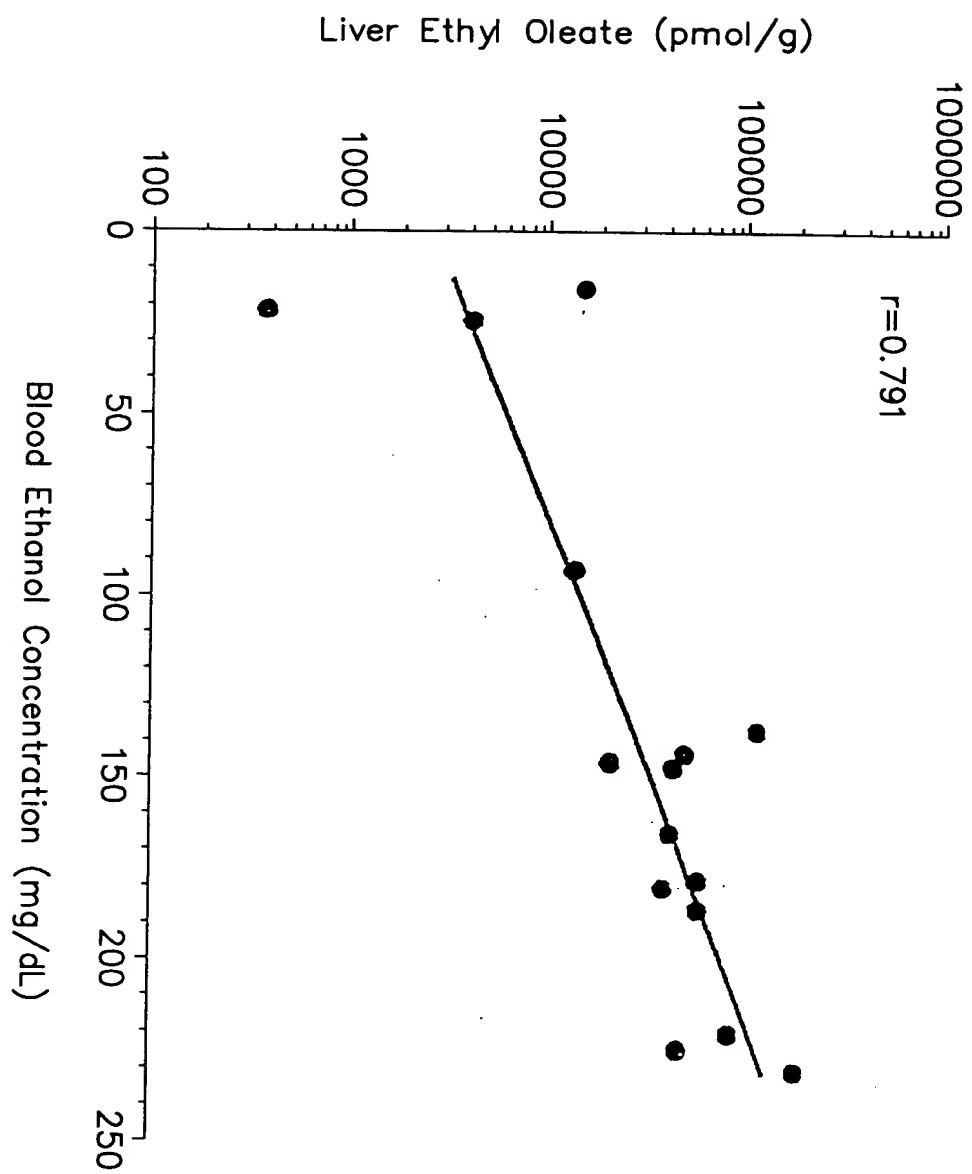


FIG. 17




FIG. 18

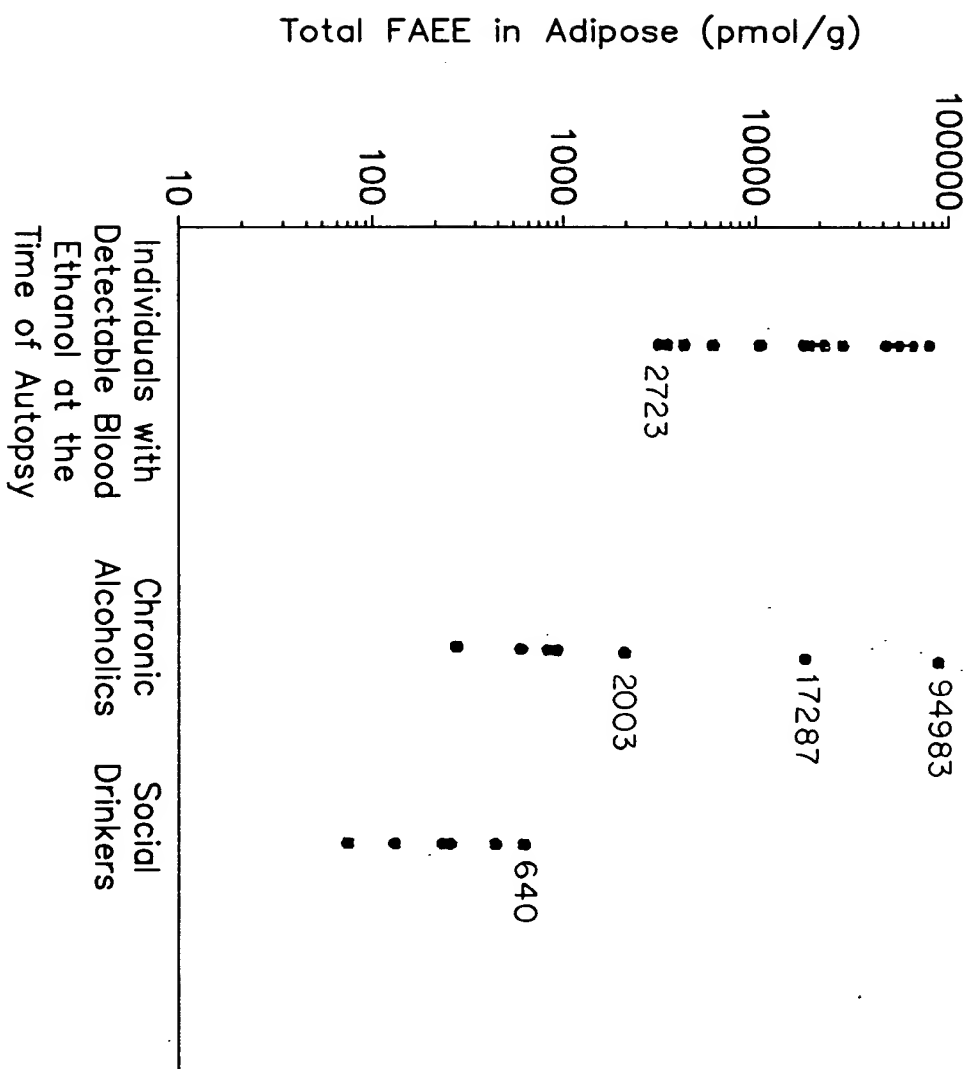


FIG. 19

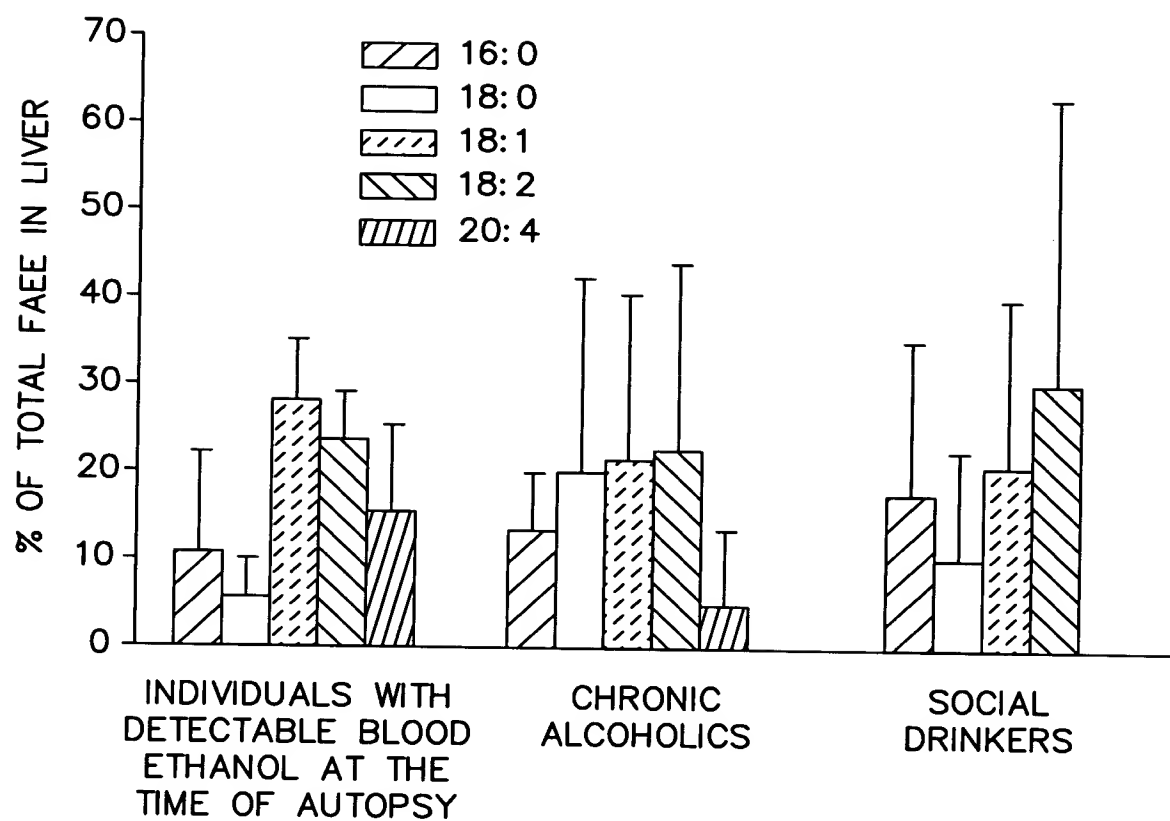


FIG. 20

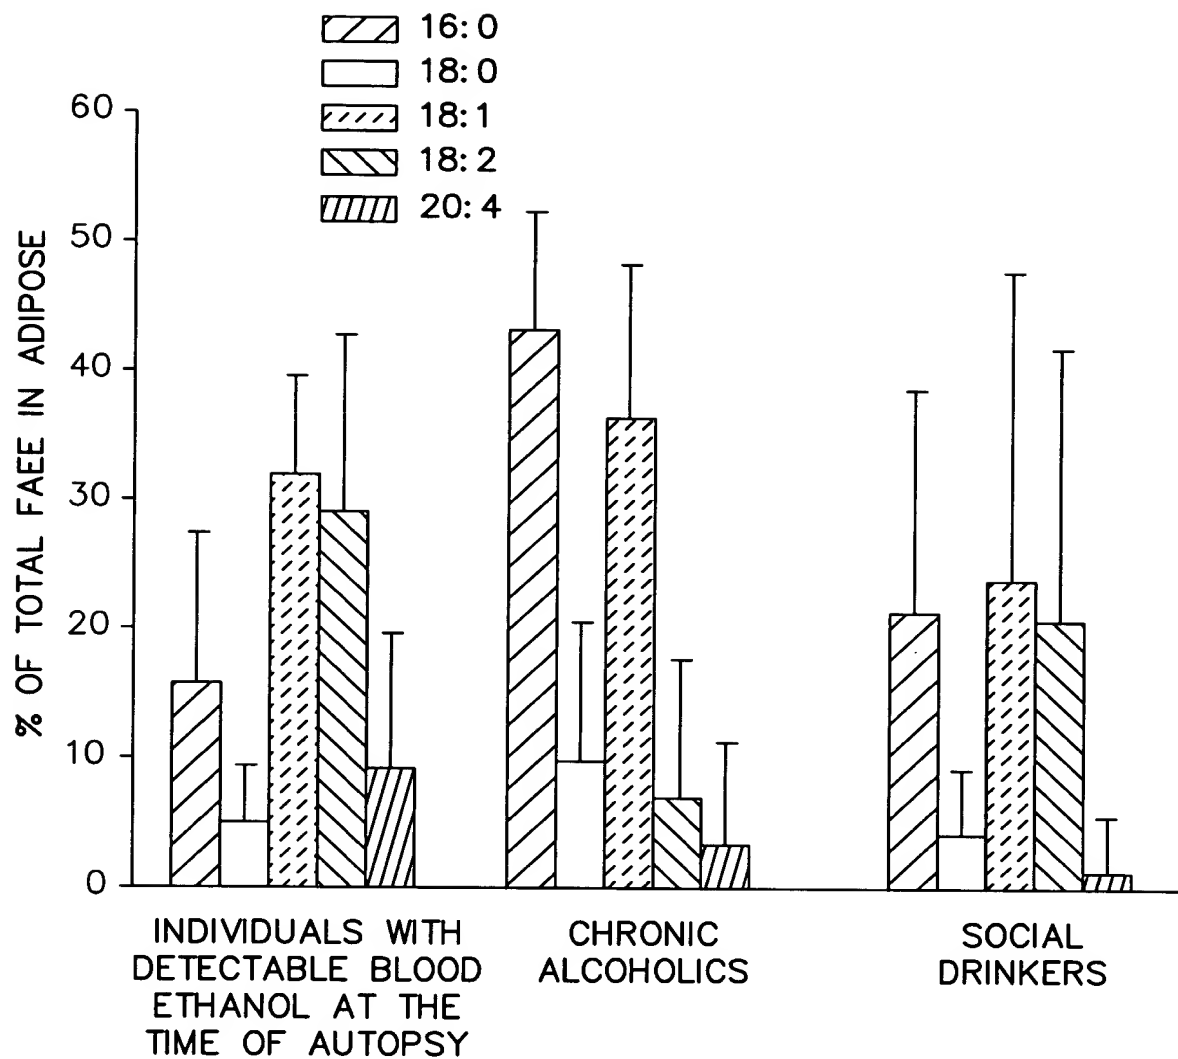


FIG. 21

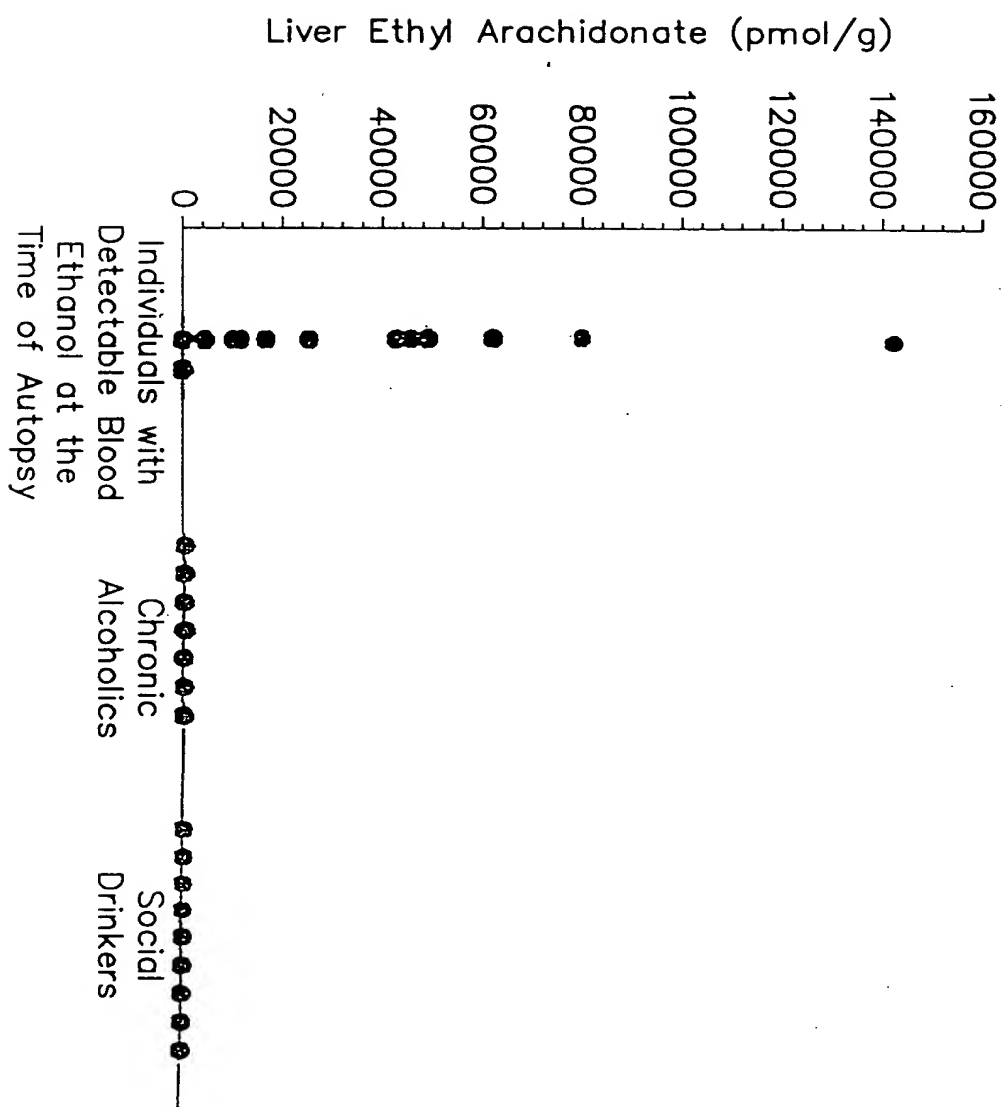


FIG. 22

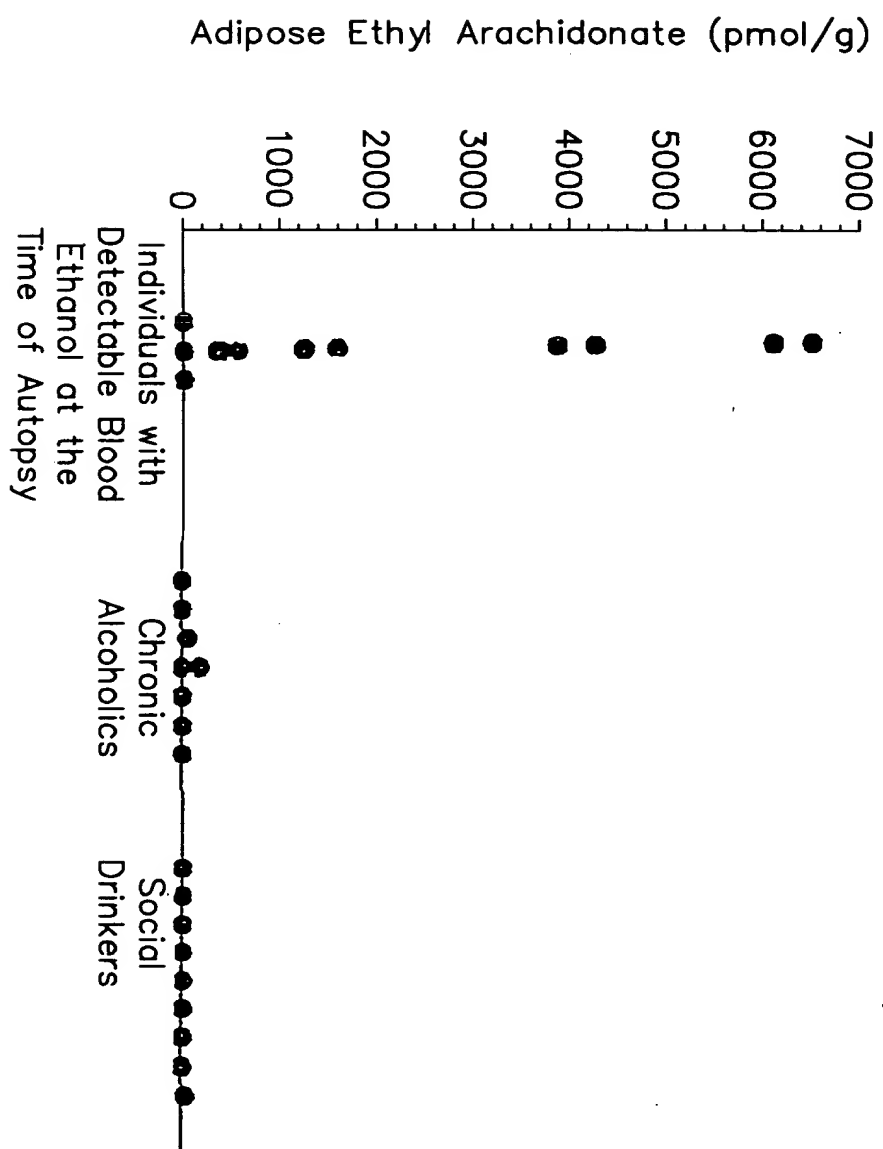


FIG. 23

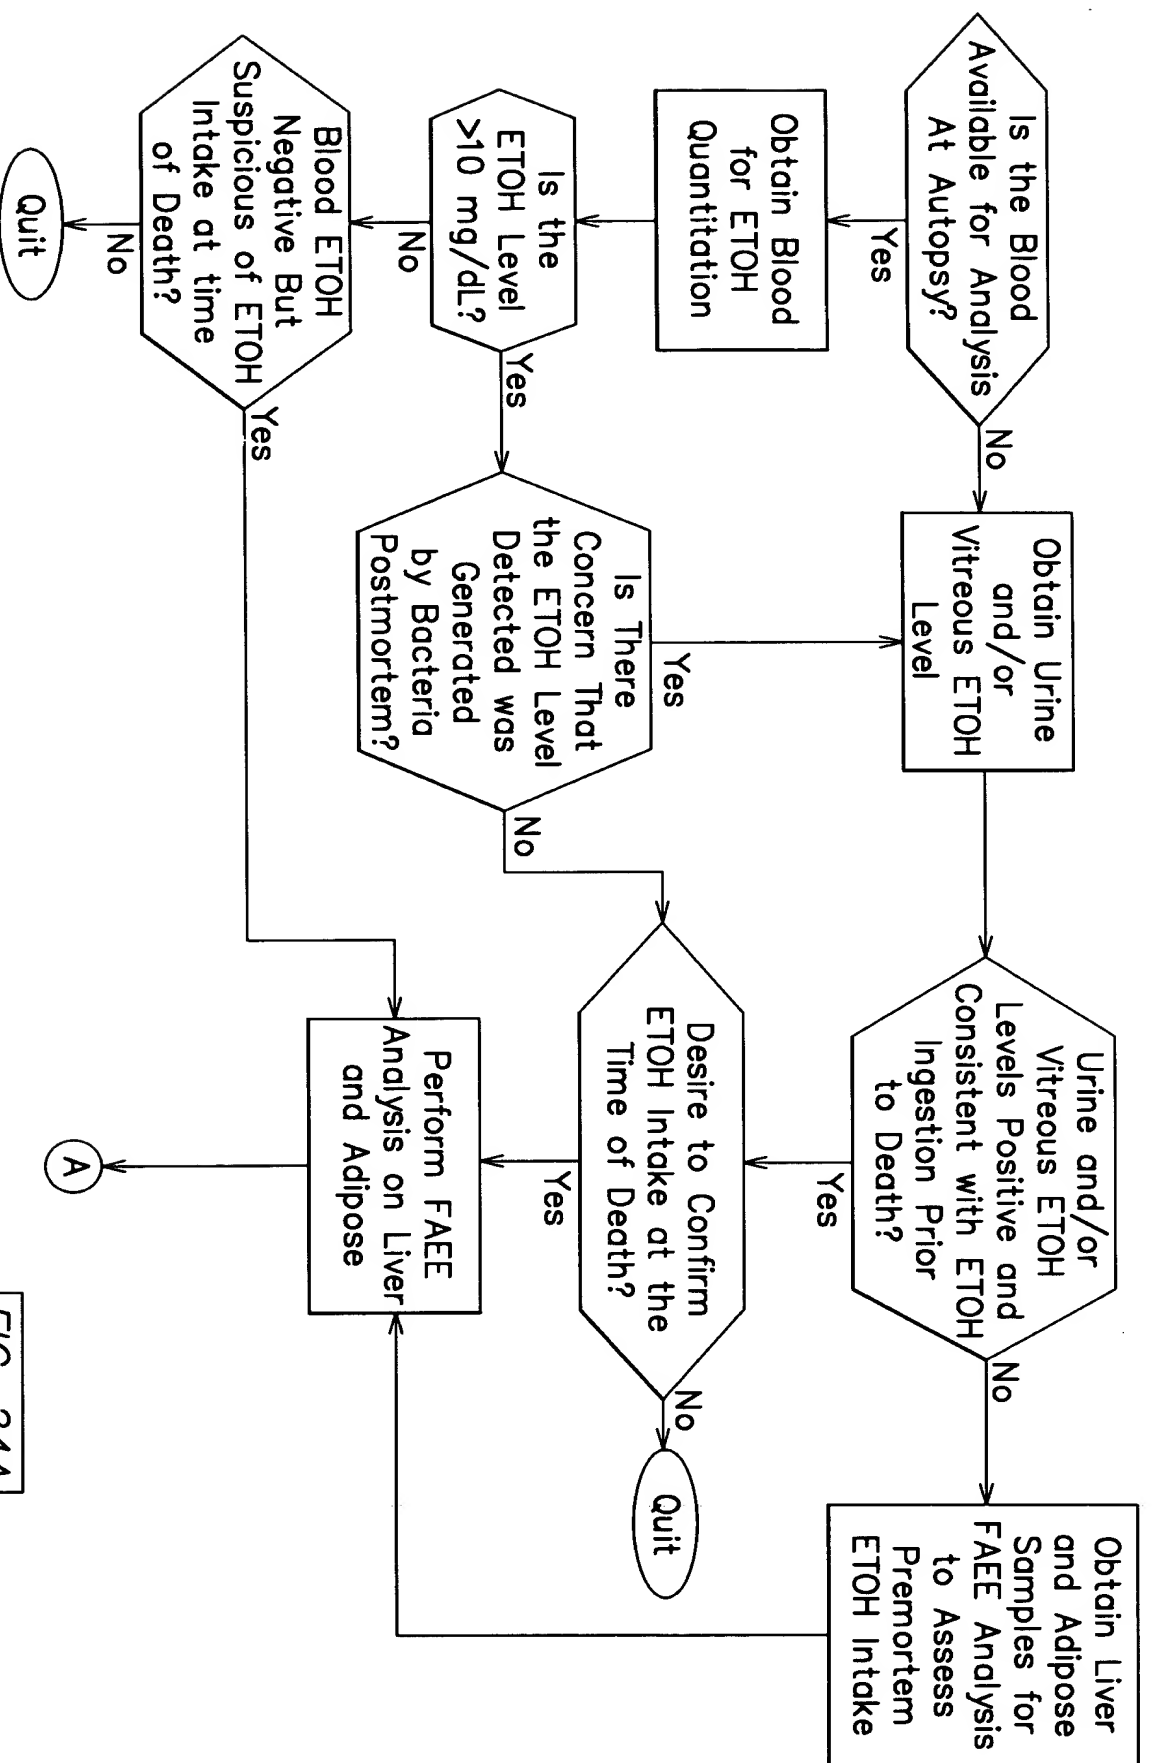


FIG. 24A

FIG. 24A
FIG. 24B

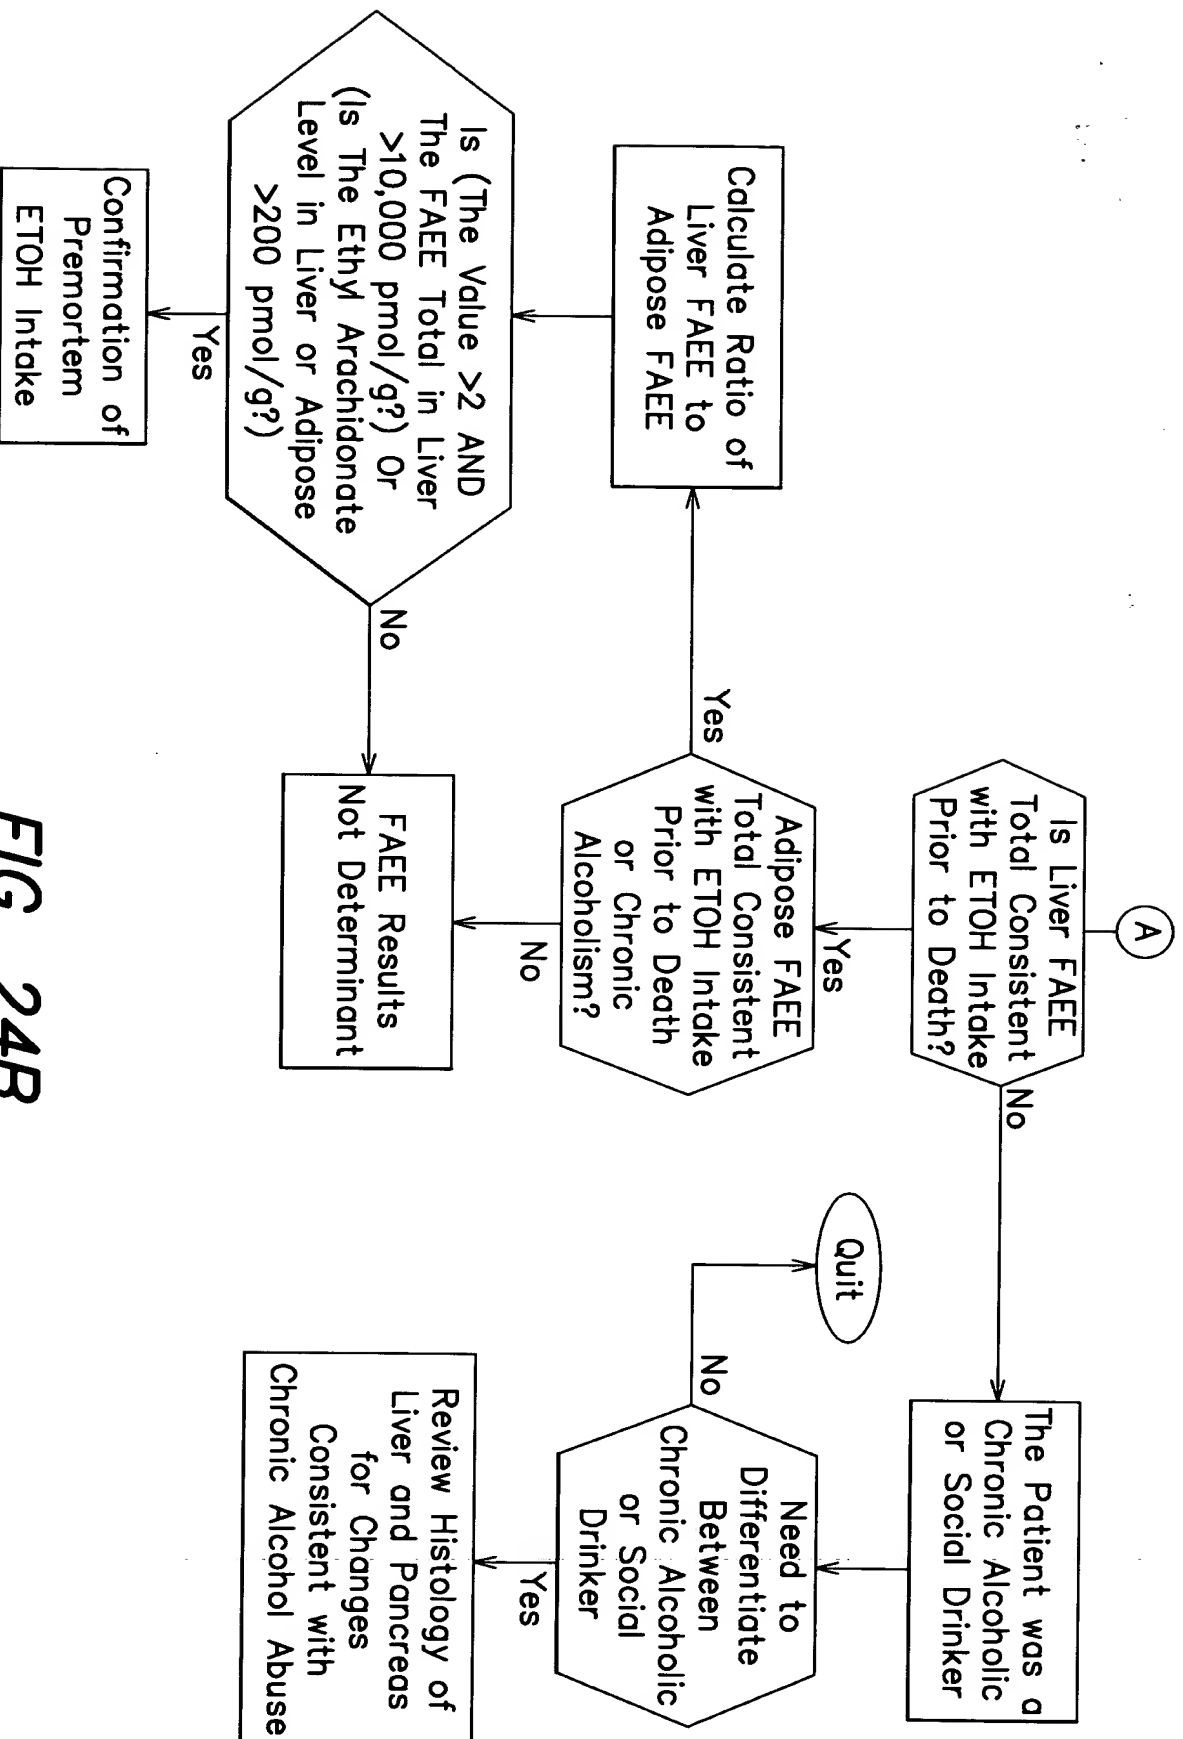


FIG. 24B